Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 033D
PDI Gage Factor: 94.7
Mean Linear Correlation Coefficient: 0.999952

Table 1: Representative Calibration Data

Applied strain (µE)	Gage Output (mV/Vexc)	Applied strain (µE)	Gage Output (mV/Vexc)
-1804.5	-5.515	518.4	1.573
-1299.2	-4.006	787.4	2.408
-826.8	-2.536	1063.0	3.239
-479.0	-1.477	1332.0	4.076
-144.4	-0.494	1607.6	4.894
229.7	0.685	2014.4	6.071

Calibration Curve

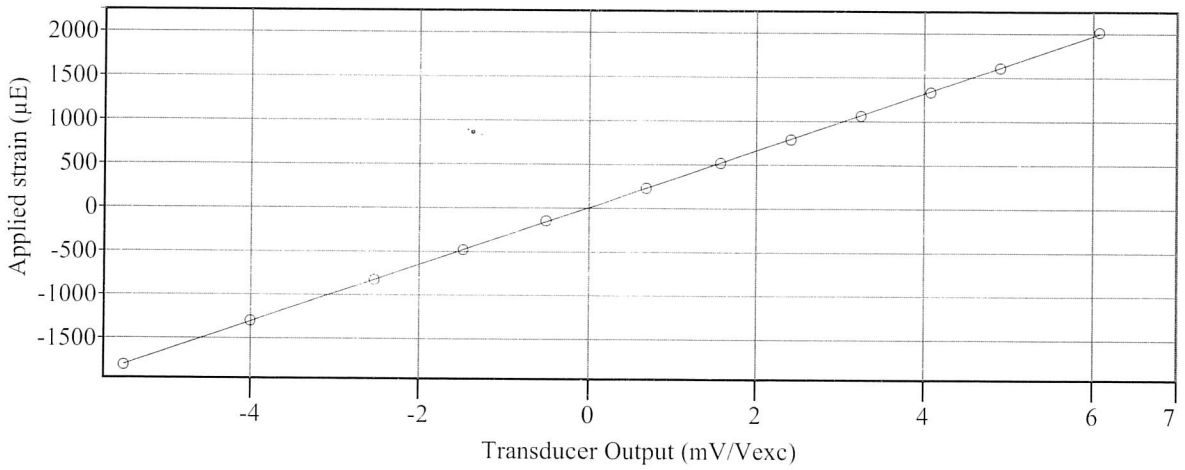

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 033D

Calibration Date: OCT 15 2026

Calibration valid 2 years

Pile Dynamics, Inc.