
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 043D
PDI Gage Factor: 93.3
Mean Linear Correlation Coefficient: 0.999983

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2053.8	-6.313	643.0	2.057
-1469.8	-4.527	971.1	3.049
-909.9	-2.765	1292.7	4.060
-498.7	-1.519	1627.3	5.087
-91.9	-0.244	2001.3	6.205
321.5	1.041		

Calibration Curve

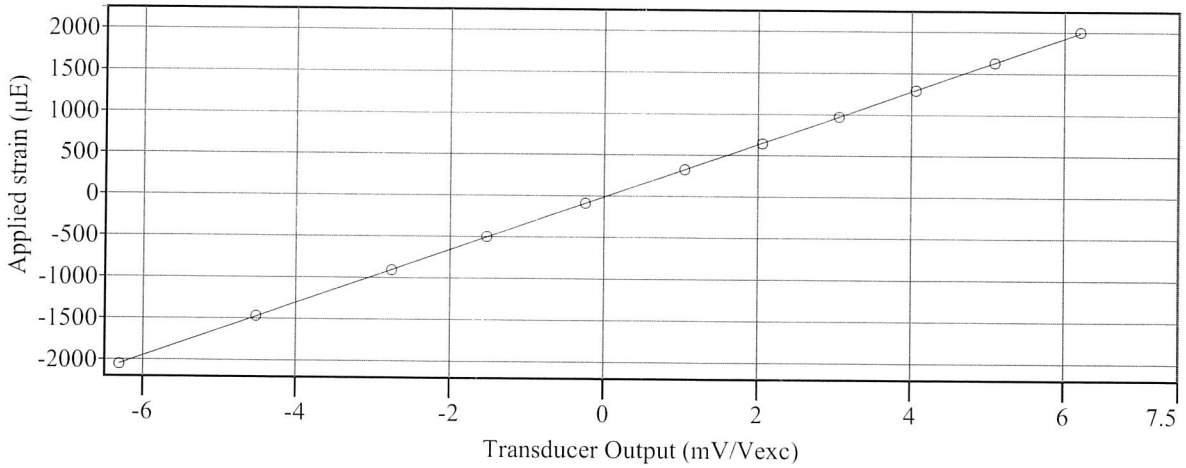

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal
Signature: Kelly Beal
PDI Gage: 043D
Calibration Date: OCT 15 2026
Calibration valid 2 years

Pile Dynamics, Inc.