
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 044D
PDI Gage Factor: 93.3
Mean Linear Correlation Coefficient: 0.999943

Table 1: Representative Calibration Data

Applied strain (µE)	Gage Output (mV/Vexc)	Applied strain (µE)	Gage Output (mV/Vexc)
-2073.5	-6.415	649.6	2.061
-1493.9	-4.621	971.1	3.057
-925.2	-2.850	1299.2	4.086
-538.1	-1.651	1647.0	5.104
-85.3	-0.255	2001.3	6.152
315.0	1.021		

Calibration Curve

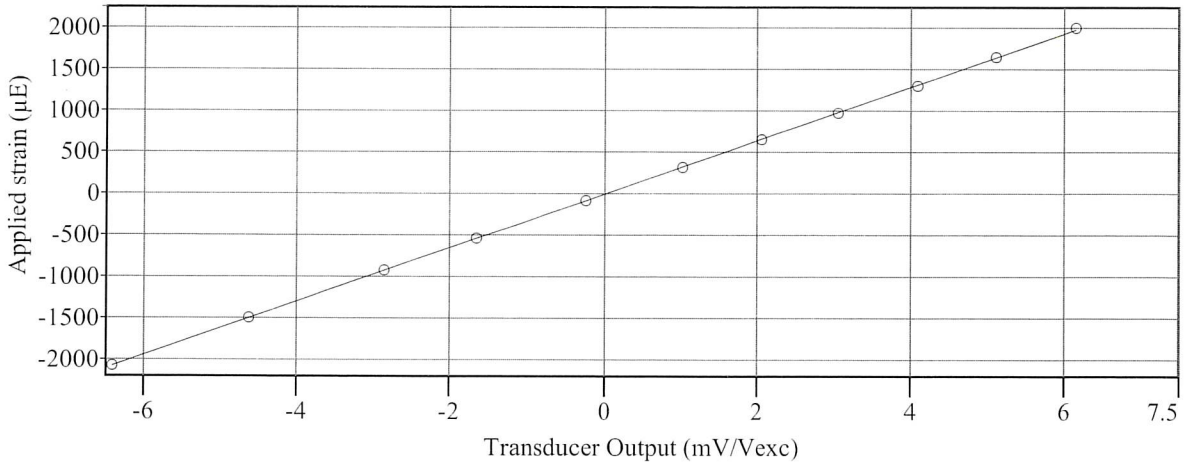

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 044D

Calibration Date: OCT 23 2026

Calibration valid 2 years

Pile Dynamics, Inc.