
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 047D
PDI Gage Factor: 91.8
Mean Linear Correlation Coefficient: 0.999965

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2099.7	-6.655	675.9	2.136
-1522.3	-4.840	1003.9	3.134
-951.4	-3.006	1325.5	4.163
-524.9	-1.669	1660.1	5.190
-98.4	-0.339	2003.5	6.226
334.6	1.045		

Calibration Curve

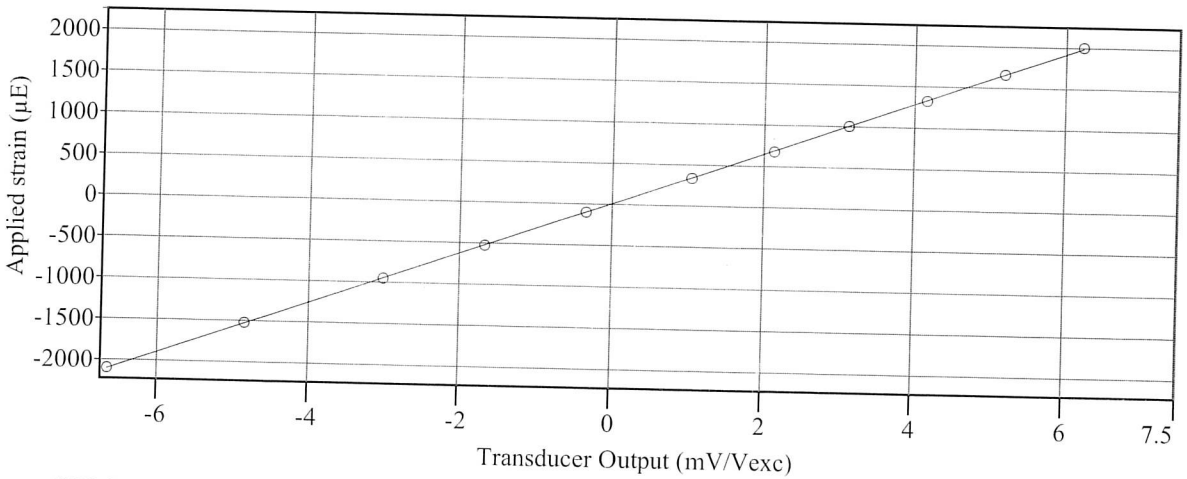

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal
Signature: Kelly Beal
PDI Gage: 047D
Calibration Date: OCT 15 2026
Calibration valid 2 years

Pile Dynamics, Inc.