


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

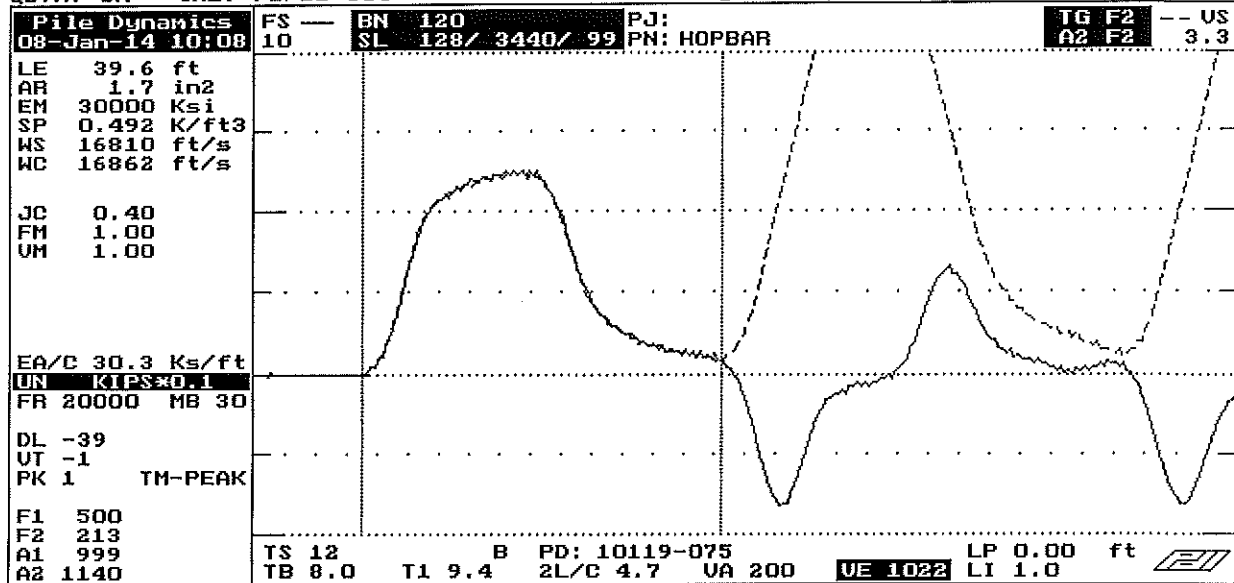

ACCEPT SQ-OFF FL-OFF PR-OFF



contact File Dynamics USA
 with your questions
 tel USA - 216 - 831- 6131
 fax USA - 216 - 831- 0916

UMX= 4.1 FMX= 63 AMX= 129
 EMX= 0.2 MEX= 123 FUP= 1.00

ACCELEROMETER CALIBRATION N.I.S.T. Traceable

SERIAL NUMBER: 10119

CALIBRATION FACTOR: 1140 G/v

PAK-(#5880): DATE: 8-Jan-14

PDA OPERATOR: Erik S. [Signature]

<-AT:PIEZORESISTIVE

OP: erik [ver:4.05]

AT:PIEZOELECTRIC->