
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 215D
PDI Gage Factor: 95.5
Mean Linear Correlation Coefficient: 0.999978

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2075.7	-6.250	669.3	2.065
-1502.6	-4.503	984.3	3.026
-918.6	-2.767	1312.3	4.030
-505.2	-1.521	1653.5	5.033
-85.3	-0.229	2001.3	6.053
334.6	1.055		

Calibration Curve

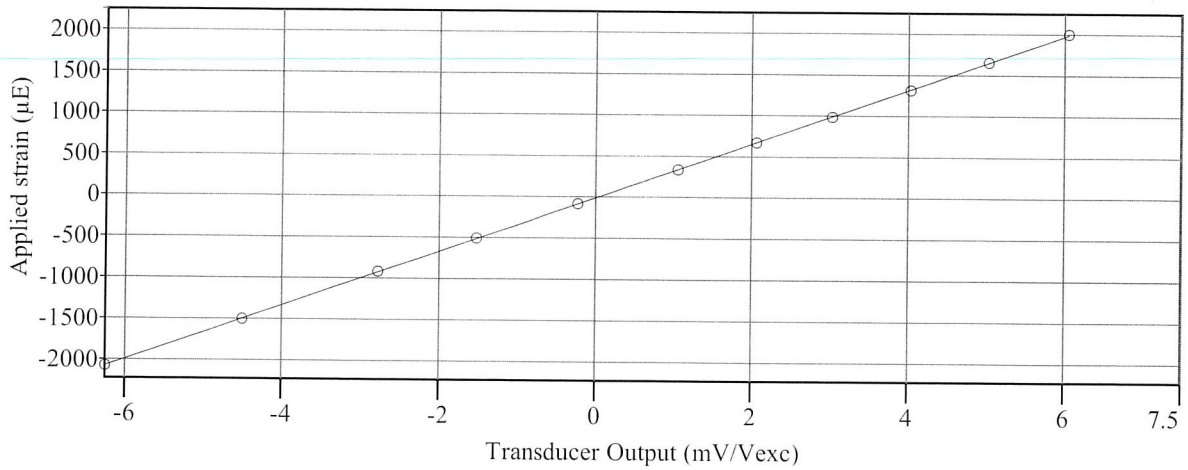

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: Kelly Beal

PDI Gage: 215D

Calibration Date: OCT 15 2026

Calibration valid 2 years

Pile Dynamics, Inc.