
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 360B
PDI Gage Factor: 91.8
Mean Linear Correlation Coefficient: 0.999916

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2231.0	-7.056	446.2	1.439
-1719.2	-5.436	850.8	2.699
-1194.2	-3.791	1168.0	3.713
-689.0	-2.189	1485.1	4.669
-315.0	-1.005	1811.0	5.632
19.7	0.083	2001.3	6.205

Calibration Curve

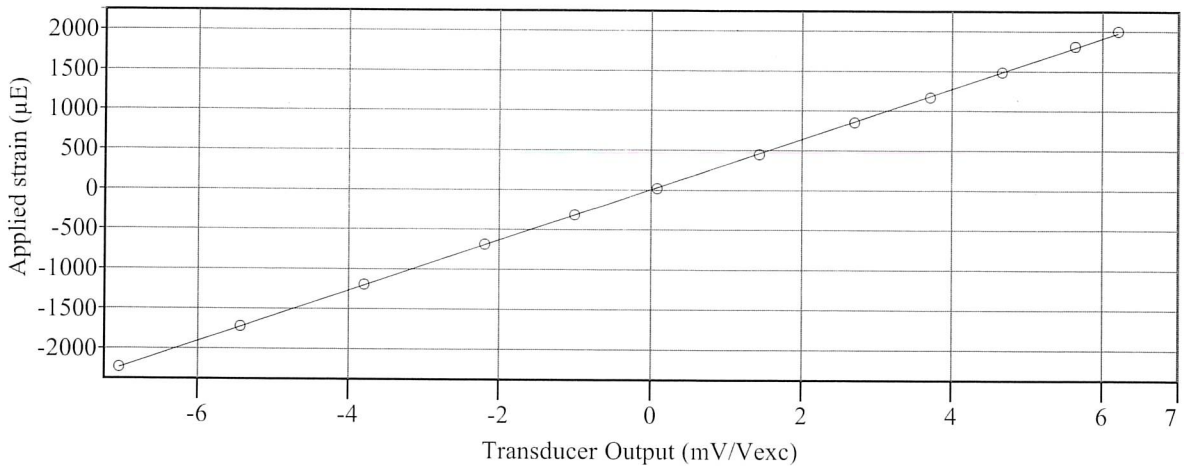

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: Kelly Beal

PDI Gage: 360B

Calibration Date: OCT 21 2026

Calibration valid 2 years

Pile Dynamics, Inc.