
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 668B
PDI Gage Factor: 92.2
Mean Linear Correlation Coefficient: 0.999862

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1896.3	-6.023	669.3	2.105
-1378.0	-4.408	1010.5	3.165
-879.3	-2.800	1312.3	4.096
-459.3	-1.482	1633.9	5.047
-137.8	-0.459	2007.9	6.147
258.1	0.805		

Calibration Curve

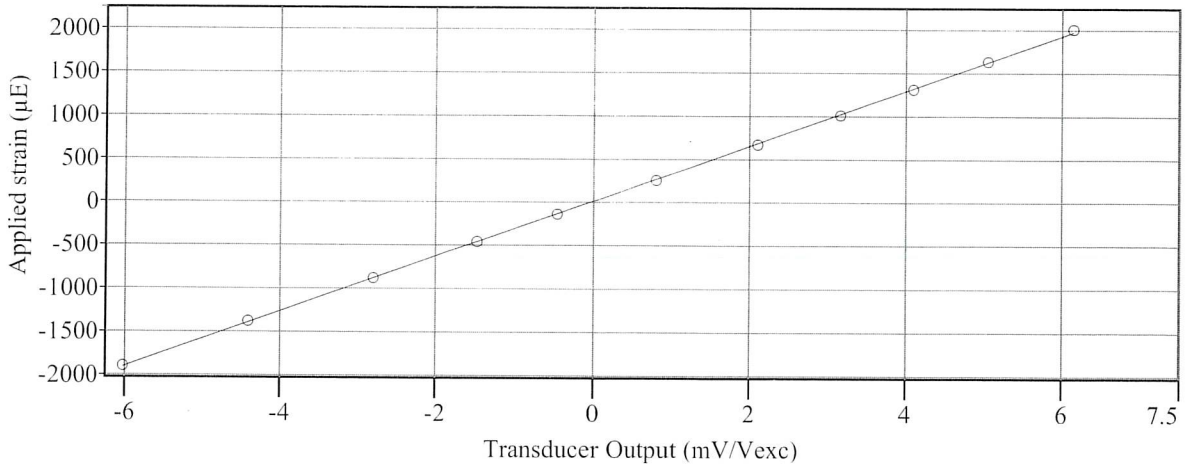

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 668B

Calibration Date: OCT 19 2026

Calibration valid 2 years

Pile Dynamics, Inc.