Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 711B
PDI Gage Factor: 138.3
Mean Linear Correlation Coefficient: 0.999917

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2023.8	-4.363	414.2	0.769
-1606.2	-3.458	766.3	1.527
-1224.9	-2.619	1150.9	2.330
-837.1	-1.800	1560.8	3.159
-439.8	-0.982	1941.0	3.948
36.4	-0.022		

Calibration Curve

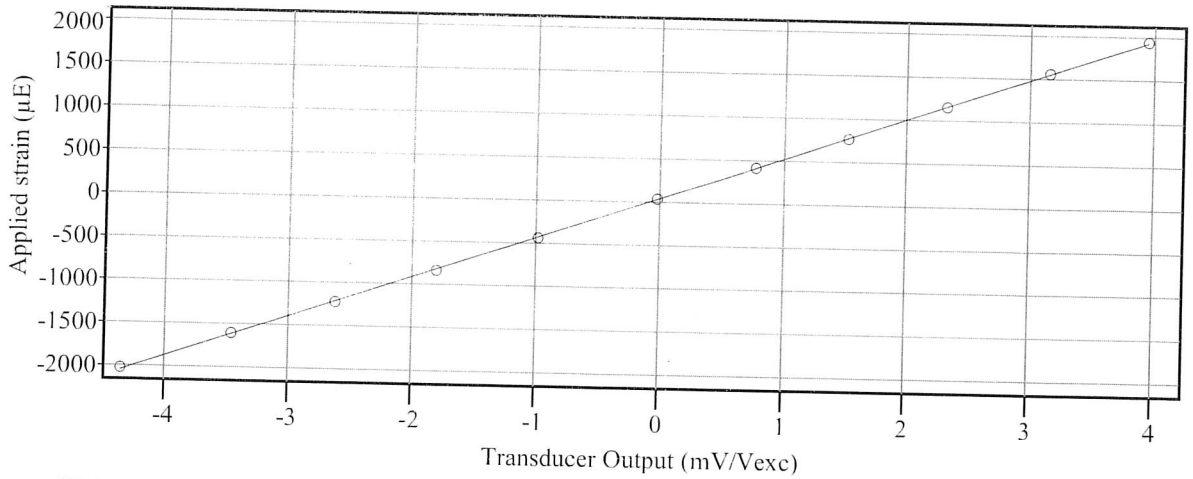

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: Kelly Beal

PDI Gage: 711B

Calibration Date: 10/21/2026 9:04:14 AM

Calibration valid 2 years

Pile Dynamics, Inc.