


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

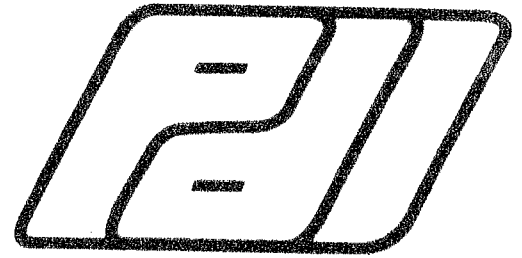


Serial No: K0281 Temperature: 23.5 °C
Model: KICHER PR Humidity: 30%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

357.6 mv/5000g
(71.5 μ v/g)
R²: 0.999947 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 09Oct2026

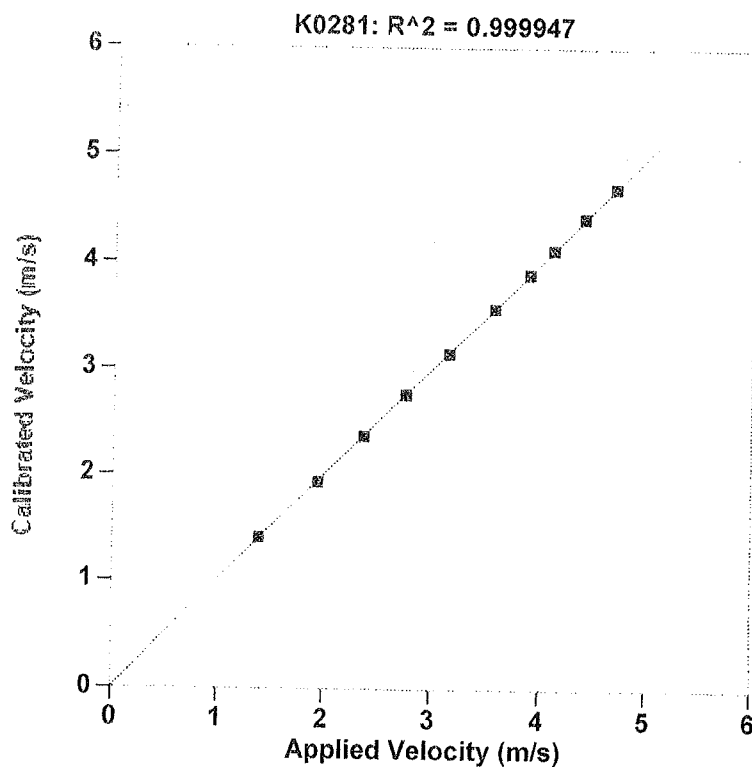

Reference Velocity	S/N K0281 Velocity
m/s	m/s
1.397	1.399
1.941	1.929
2.365	2.359
2.758	2.752
3.157	3.142
3.564	3.565
3.890	3.891
4.114	4.117
4.409	4.418
4.696	4.703
Maximum Acceleration: 1014 g's	