Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K1000	**Temperature:**	22.7 °C
Model:	KICHER PR	**Humidity:**	40%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


324.5 mv/5000g
(64.9 µv/g)
R^2: 0.999966 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: 26Sep2026

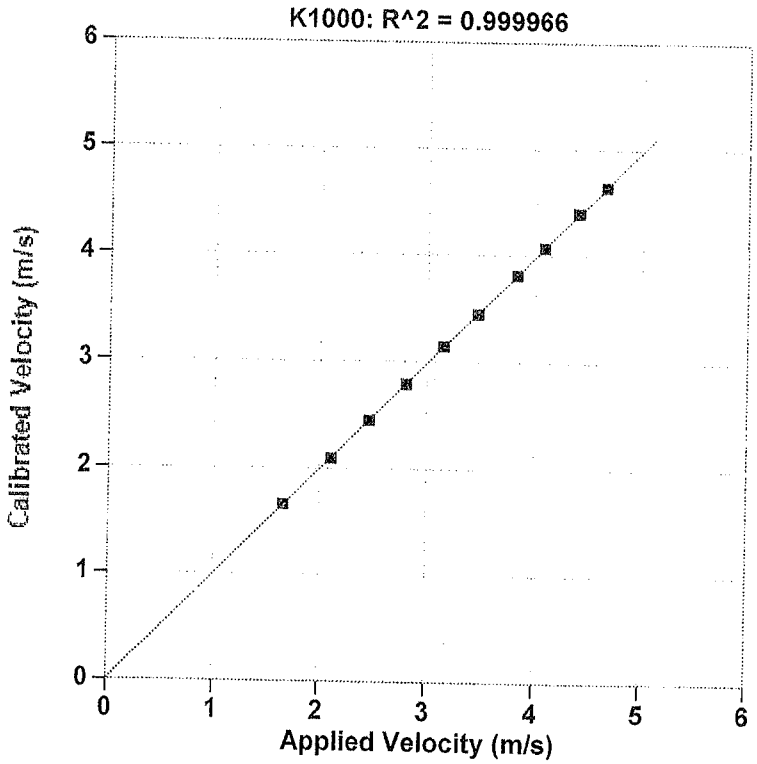

Reference Velocity	S/N K1000 Velocity
m/s	m/s
1.655	1.660
2.106	2.099
2.454	2.450
2.803	2.795
3.148	3.149
3.460	3.455
3.819	3.819
4.080	4.077
4.393	4.404
4.650	4.653

Maximum Acceleration: 1011 g's