


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

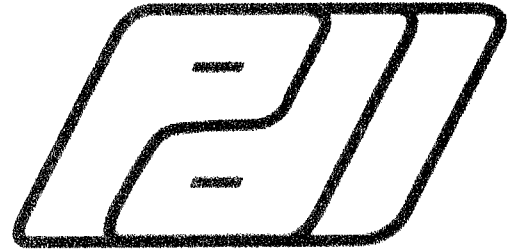

Serial No: K10166 Temperature: 23.1 °C

Model: KICHER PR Humidity: 39%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

390.2 mv/5000g

(78.0 μ v/g)

R²: 0.999995 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 15Oct2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

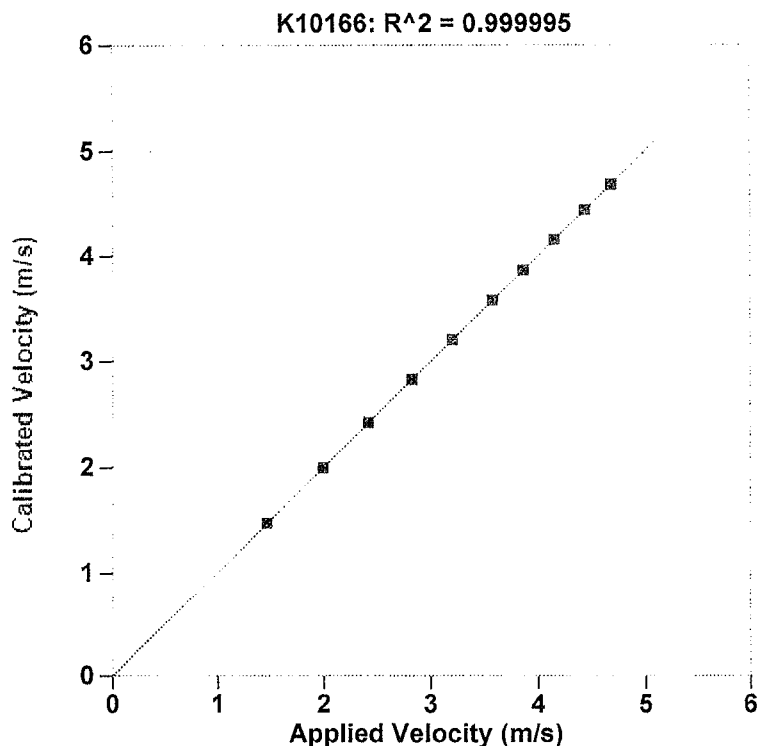

Reference Velocity	S/N K10166 Velocity
m/s	m/s
1.461	1.465
1.993	1.991
2.418	2.420
2.829	2.828
3.205	3.206
3.578	3.581
3.863	3.863
4.152	4.152
4.438	4.439
4.687	4.683

Maximum Acceleration: 1043 g's