


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

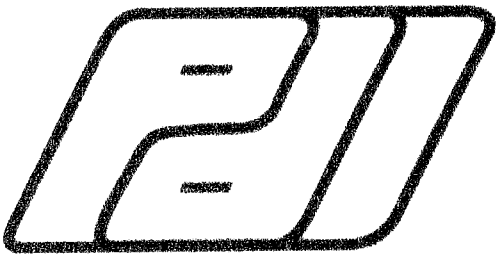


Serial No: K10548 Temperature: 22.9 °C
Model: KICHER PR Humidity: 39%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

403.0 mv/5000g
(80.6 μv/g)
R^2: 0.999986 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 15Oct2026

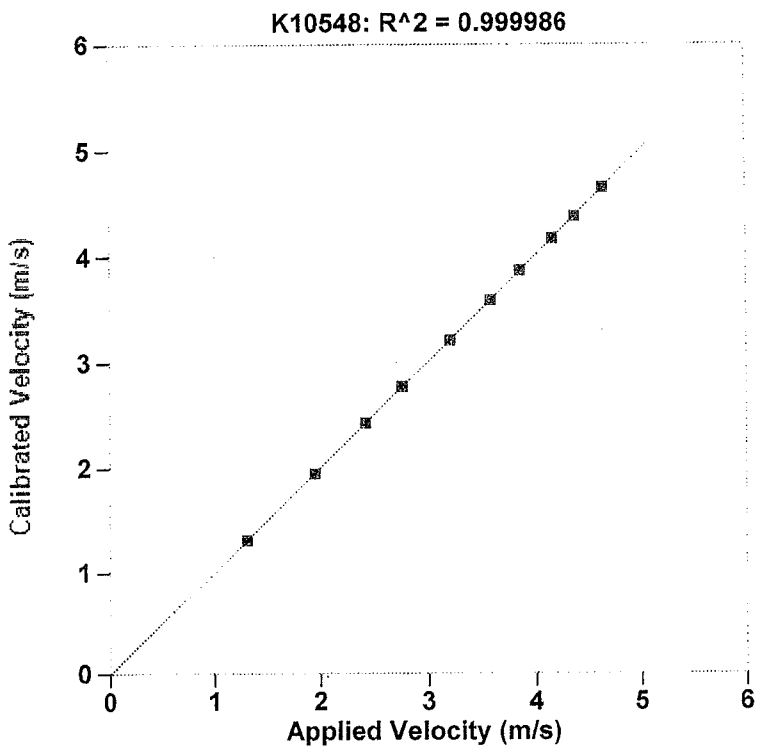

Reference Velocity	S/N K10548 Velocity
m/s	m/s
1.306	1.307
1.950	1.944
2.420	2.423
2.764	2.767
3.205	3.208
3.583	3.584
3.861	3.863
4.159	4.163
4.380	4.372
4.648	4.647
Maximum Acceleration: 1032 g's	