


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

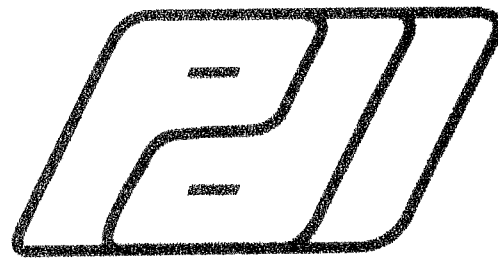

Serial No: K10875 Temperature: 21.9 °C

Model: KICHER PR Humidity: 40%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

391.3 mv/5000g


(78.3 μ v/g)

R²: 0.999992 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Calibration valid 2 years

From: 26Sep2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

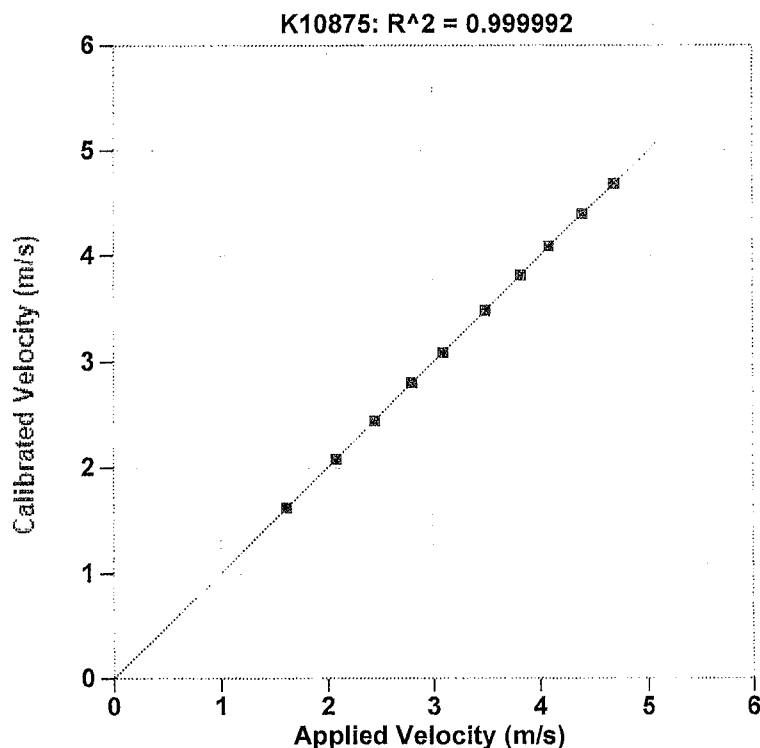

Reference Velocity	S/N K10875 Velocity
m/s	m/s
1.615	1.618
2.083	2.081
2.450	2.444
2.800	2.803
3.093	3.090
3.488	3.491
3.822	3.822
4.092	4.094
4.407	4.408
4.698	4.697

Maximum Acceleration: 1019 g's