


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

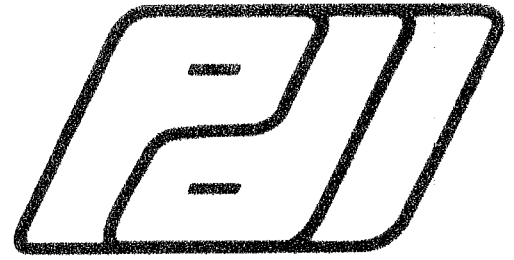

Serial No: K11546 Temperature: 21.8 °C

Model: KICHER PR Humidity: 41%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

426.1 mv/5000g


(85.2 μ v/g)

R²: 0.999972 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 26Sep2026

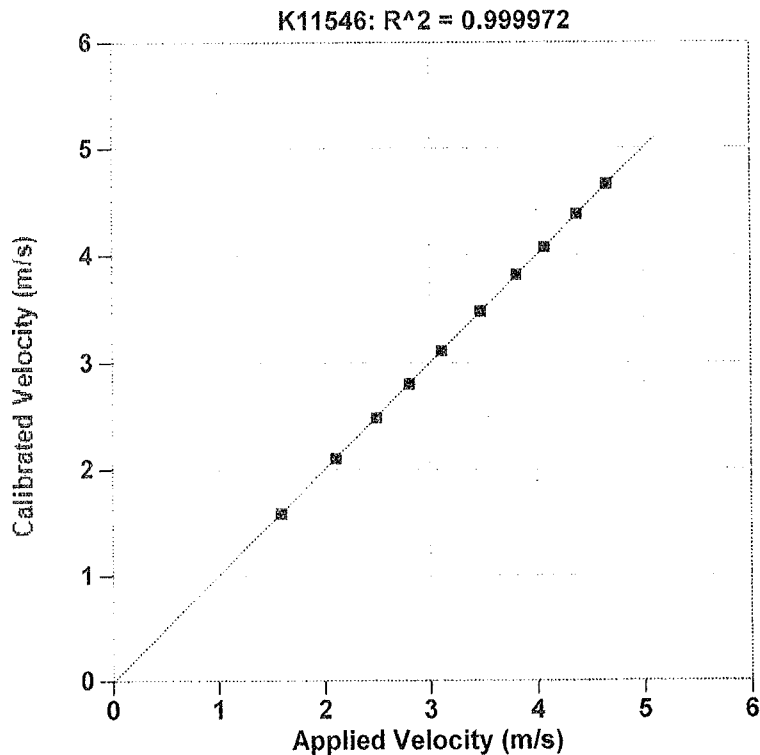

Reference Velocity	S/N K11546 Velocity
m/s	m/s
1.580	1.579
2.106	2.101
2.491	2.485
2.805	2.799
3.112	3.110
3.470	3.479
3.812	3.819
4.073	4.073
4.381	4.380
4.664	4.664

Maximum Acceleration: 1014 g's