


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

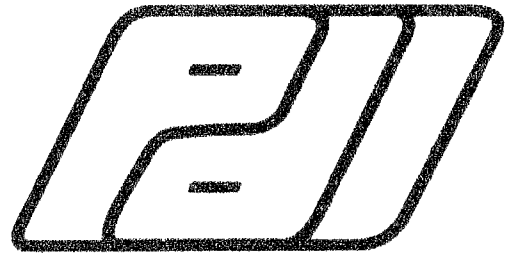

Serial No: K14817 Temperature: 22.3 °C

Model: KICHER PR Humidity: 39%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

410.5 mv/5000g


(82.1 μ v/g)

R²: 0.999975 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Calibration valid 2 years

From: 26Sep2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

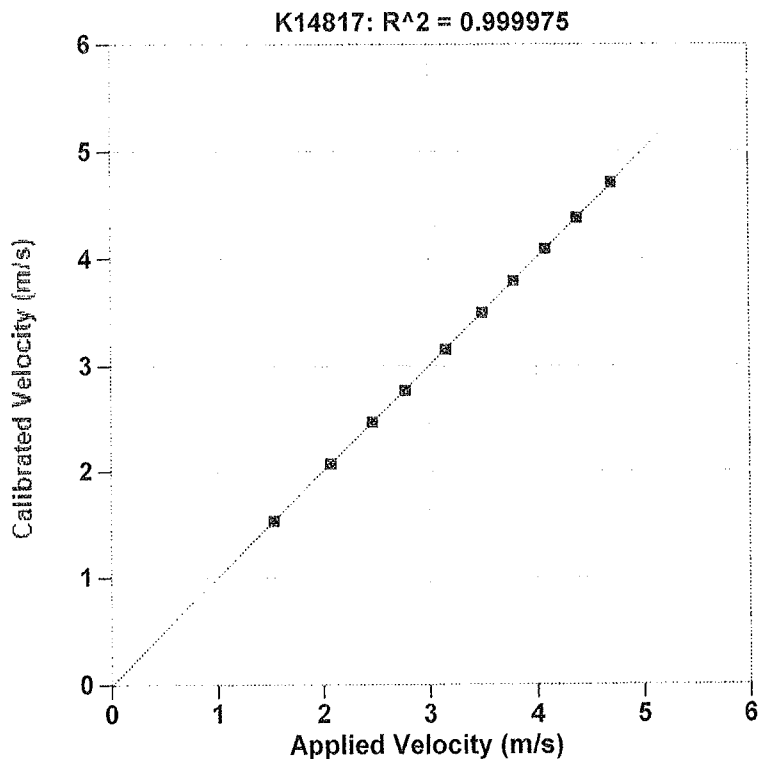

Reference Velocity	S/N K14817 Velocity
m/s	m/s
1.534	1.534
2.071	2.071
2.463	2.467
2.771	2.763
3.157	3.154
3.501	3.496
3.797	3.793
4.084	4.085
4.381	4.382
4.701	4.711

Maximum Acceleration: 1020 g's