

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15567 Temperature: 23.5 °C
Model: KICHER PR Humidity: 37%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

337.9 mv/5000g
(67.6 μv/g)
R^2: 0.999986 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt


Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years
From: **OCT 15 2026**

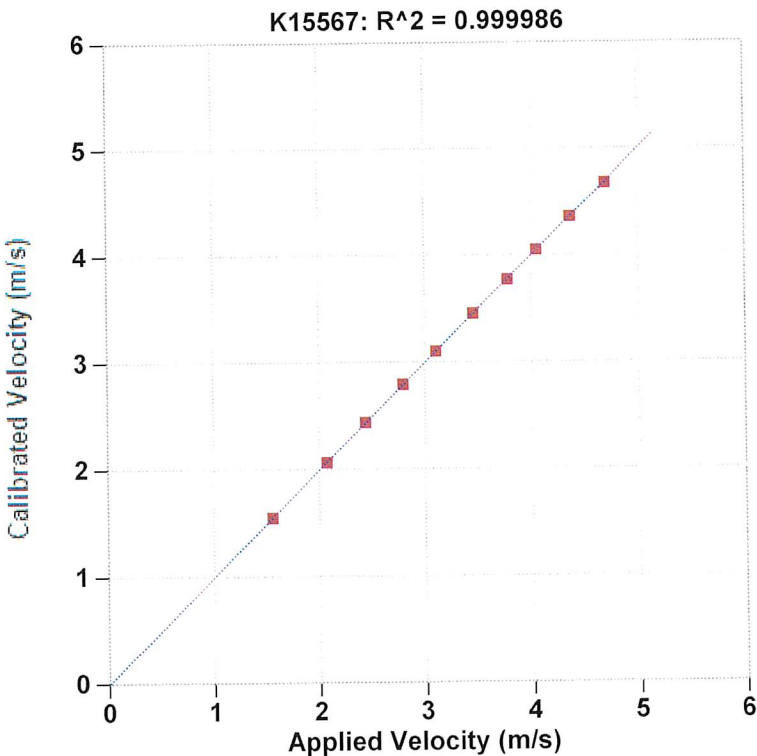

Reference Velocity	S/N K15567 Velocity
m/s	m/s
1.547	1.550
2.069	2.068
2.436	2.441
2.791	2.795
3.102	3.102
3.455	3.454
3.779	3.772
4.046	4.050
4.360	4.361
4.677	4.675
Maximum Acceleration: 1011 g's	