

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15568 Temperature: 24.0 °C
Model: KICHER PR Humidity: 35%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

386.4 mv/5000g
(77.3 μv/g)
R^2: 0.999942 [Chip programmed]


Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years
From: OCT 15 2026

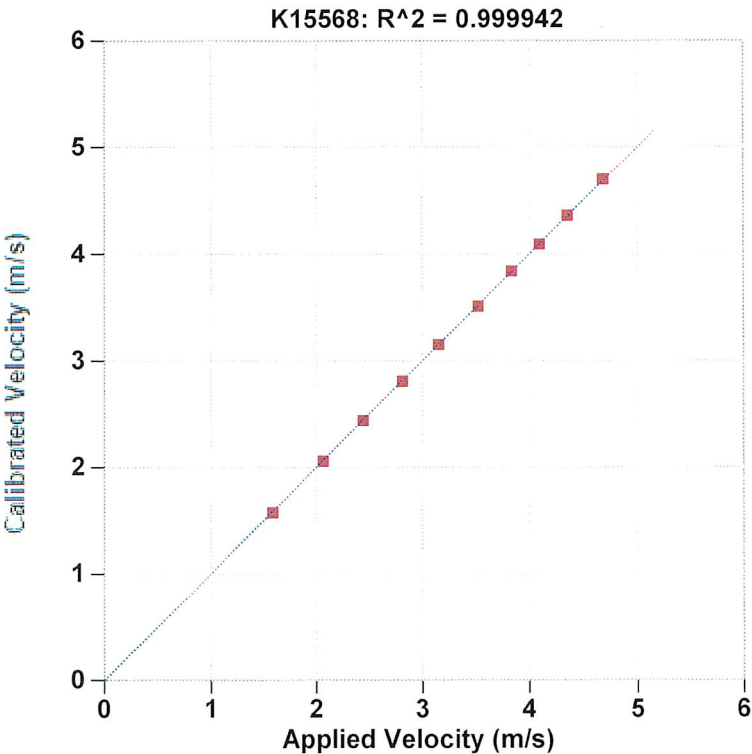

Reference Velocity	S/N K15568 Velocity
m/s	m/s
1.580	1.575
2.062	2.056
2.445	2.437
2.812	2.805
3.150	3.152
3.522	3.512
3.836	3.841
4.101	4.096
4.361	4.366
4.691	4.705

Maximum Acceleration: 1013 g's