Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15626	**Temperature:**	22.6 °C
Model:	KICHER PR	**Humidity:**	24%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


411.2 mv/5000g
(82.2 µv/g)
R^2: 0.999975 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: OCT 23 2026

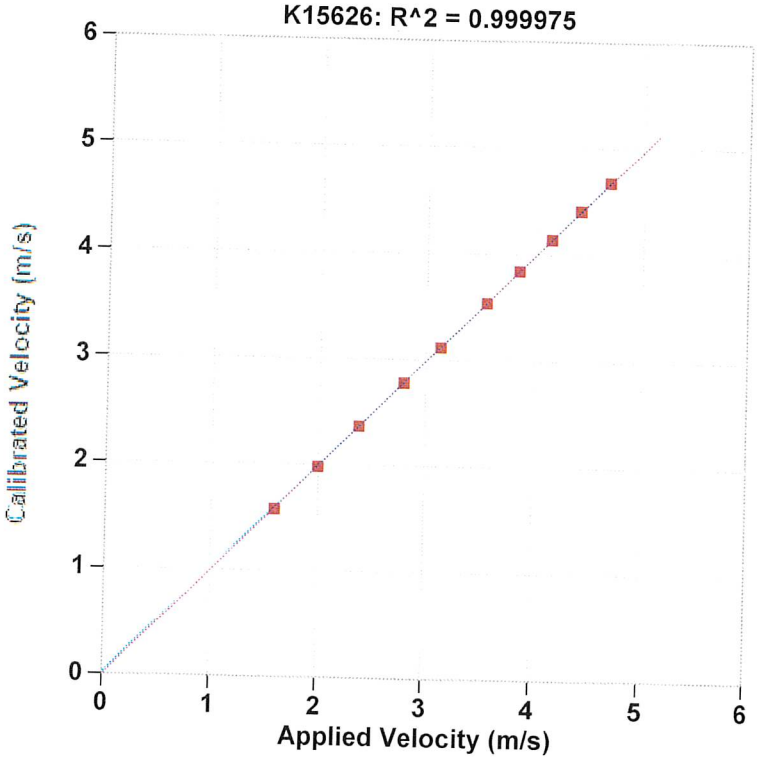

Reference Velocity	S/N K15626 Velocity
m/s	m/s
1.583	1.575
1.986	1.980
2.367	2.365
2.784	2.779
3.124	3.119
3.546	3.545
3.848	3.847
4.145	4.147
4.412	4.419
4.683	4.689

Maximum Acceleration: 1054 g's