

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15641 Temperature: 22.4 °C
Model: KICHER PR Humidity: 26%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

403.3 mv/5000g
(80.7 μv/g)
R^2: 0.999978 [Chip programmed]


Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years
OCT 19 2026
From: _____

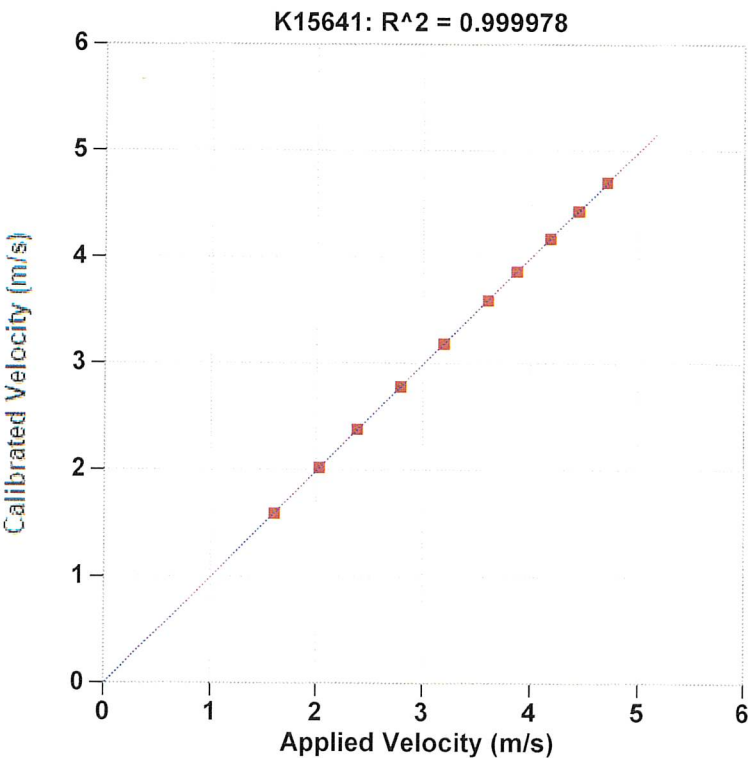

Reference Velocity	S/N K15641 Velocity
m/s	m/s
1.594	1.589
2.018	2.019
2.380	2.381
2.783	2.778
3.186	3.184
3.599	3.592
3.865	3.862
4.173	4.173
4.429	4.430
4.691	4.702

Maximum Acceleration: 1057 g's