

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15642      Temperature: 22.4 °C  
Model: KICHER PR      Humidity: 26%  
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

417.3 mv/5000g  
(83.5 μv/g)  
R^2: 0.999995 [Chip programmed]

Ref Acc 1: 85363!      Cal on: 14Nov2025  
1000 g's/volt  
Ref Acc 2: 85382!      Cal on: 24Nov2025  
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to  
the United States National Institute of Standards and  
Technology (NIST).

Calibration valid 2 years  
OCT 19 2026

From: \_\_\_\_\_

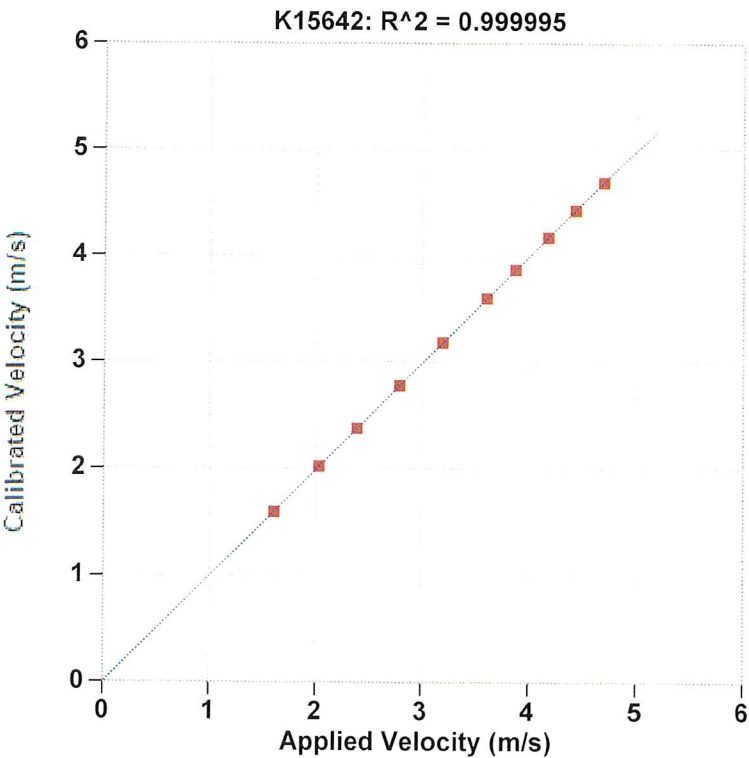

| Reference Velocity | S/N K15642 Velocity |
|--------------------|---------------------|
| m/s                | m/s                 |
| 1.594              | 1.591               |
| 2.018              | 2.023               |
| 2.380              | 2.379               |
| 2.783              | 2.782               |
| 3.186              | 3.186               |
| 3.599              | 3.600               |
| 3.865              | 3.868               |
| 4.173              | 4.172               |
| 4.429              | 4.429               |
| 4.691              | 4.689               |

Maximum Acceleration: 1057 g's