

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15643 Temperature: 22.4 °C
Model: KICHER PR Humidity: 26%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

417.7 mv/5000g
(83.5 μv/g)
R^2: 0.999977 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years
OCT 19 2026

From: _____

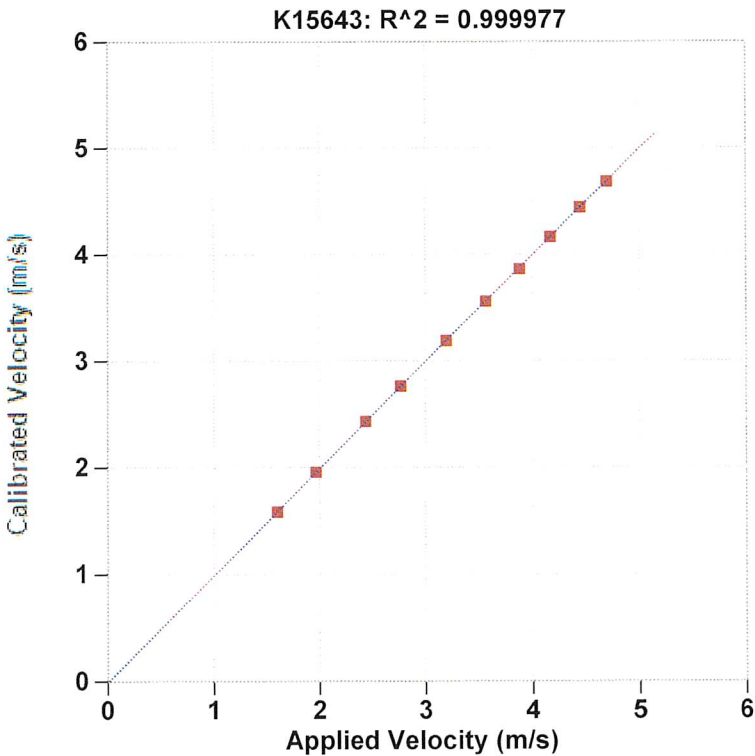

Reference Velocity	S/N K15643 Velocity
m/s	m/s
1.590	1.589
1.960	1.961
2.428	2.435
2.760	2.763
3.191	3.190
3.560	3.560
3.876	3.863
4.163	4.165
4.441	4.444
4.683	4.685

Maximum Acceleration: 1055 g's