

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15651      Temperature: 22.4 °C  
Model: KICHER PR      Humidity: 26%  
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

370.7 mv/5000g  
(74.1 μv/g)  
R^2: 0.999990 [Chip programmed]

Ref Acc 1: 85363!      Cal on: 14Nov2025  
1000 g's/volt  
Ref Acc 2: 85382!      Cal on: 24Nov2025  
958 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to  
the United States National Institute of Standards and  
Technology (NIST).

Calibration valid 2 years

From: OCT 19 2026

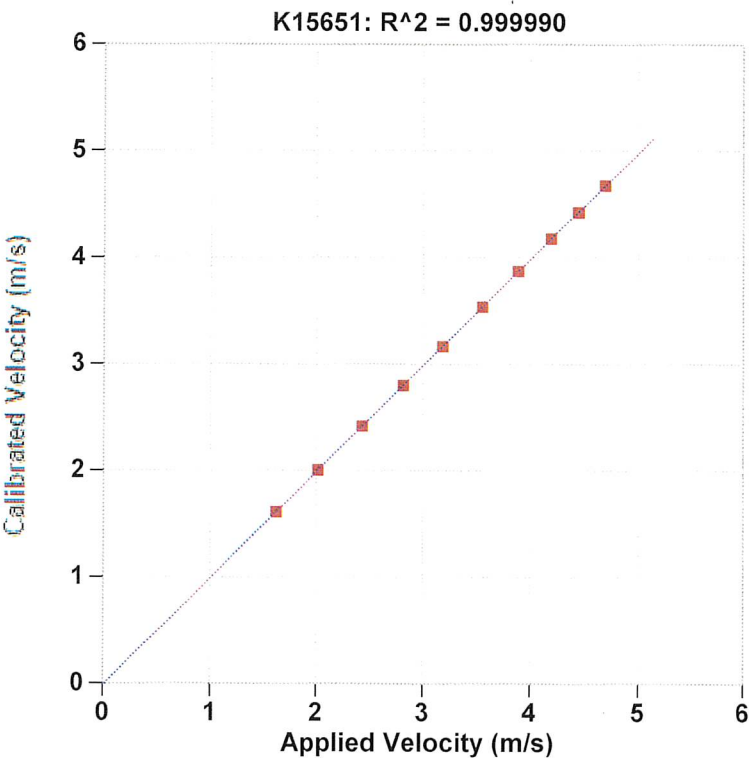

| Reference Velocity | S/N K15651 Velocity |
|--------------------|---------------------|
| m/s                | m/s                 |
| 1.611              | 1.614               |
| 2.009              | 2.012               |
| 2.421              | 2.422               |
| 2.805              | 2.804               |
| 3.171              | 3.168               |
| 3.544              | 3.543               |
| 3.881              | 3.880               |
| 4.190              | 4.187               |
| 4.438              | 4.435               |
| 4.681              | 4.688               |

Maximum Acceleration: 1057 g's