


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

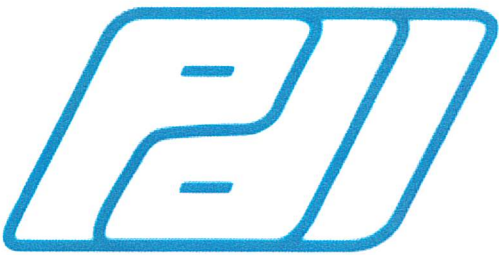

Serial No: K15652 Temperature: 22.4 °C
Model: KICHER PR Humidity: 26%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

390.9 mv/5000g
(78.2 μv/g)
R^2: 0.999981 [Chip programmed]


Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Operator: William Johnson


Signed

Calibration valid 2 years
OCT 19 2026
From: _____

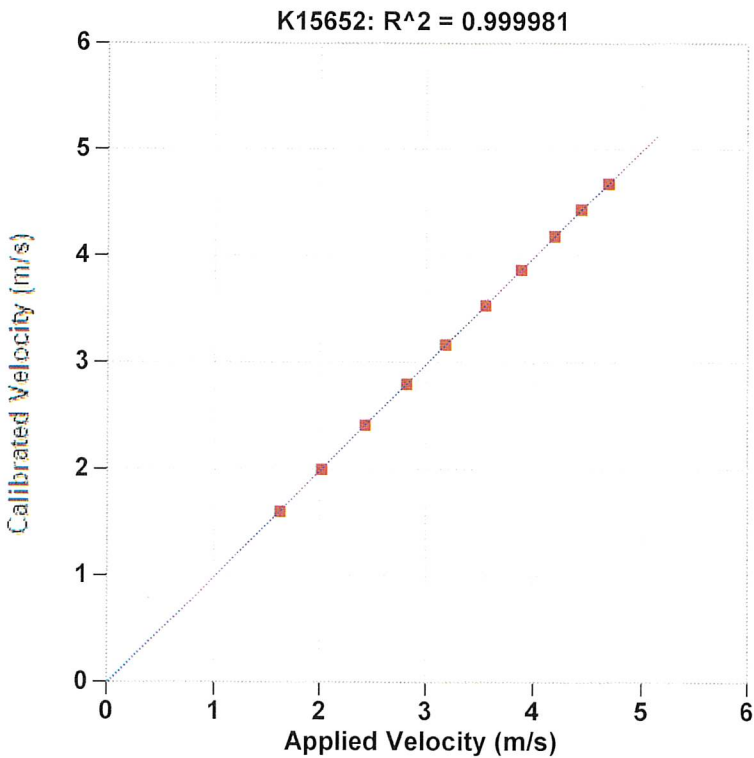

Reference Velocity	S/N K15652 Velocity
m/s	m/s
1.611	1.604
2.009	2.001
2.421	2.417
2.805	2.803
3.171	3.175
3.544	3.545
3.881	3.877
4.190	4.194
4.438	4.442
4.681	4.683

Maximum Acceleration: 1057 g's