Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15656	**Temperature:**	22.9 °C
Model:	KICHER PR	**Humidity:**	29%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

423.3 mv/5000g
(84.7 µv/g)
R^2: 0.999987 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: OCT 2 1 2026

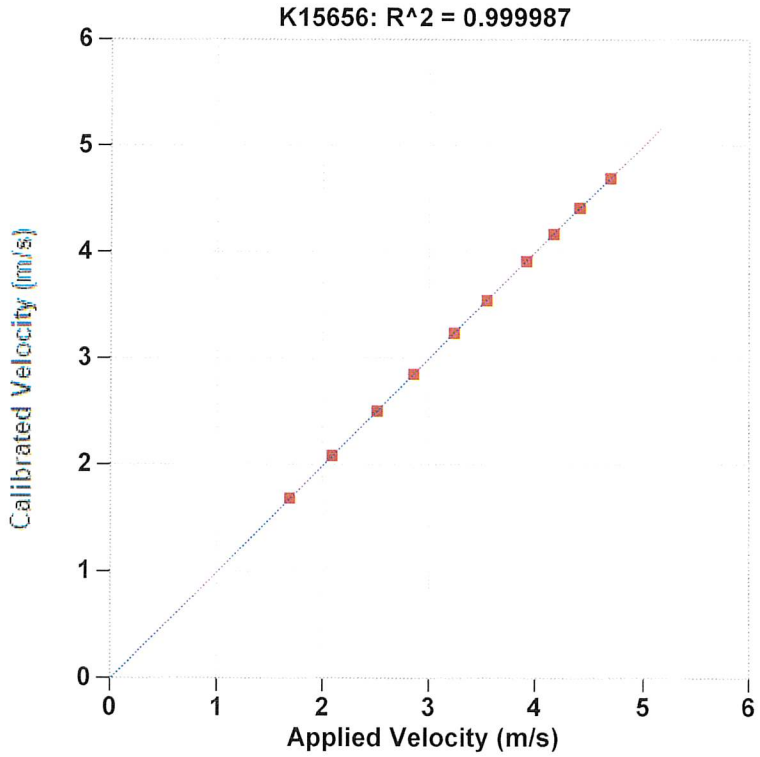

Reference Velocity	S/N K15656 Velocity
m/s	m/s
1.679	1.683
2.079	2.083
2.502	2.500
2.845	2.845
3.229	3.233
3.538	3.537
3.911	3.906
4.166	4.162
4.404	4.409
4.688	4.686

Maximum Acceleration: 1056 g's