Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15657	**Temperature:**	23.1 °C
Model:	KICHER PR	**Humidity:**	28%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

376.3 mv/5000g
(75.3 µv/g)
R^2: 0.999984 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: OCT 2 1 2026

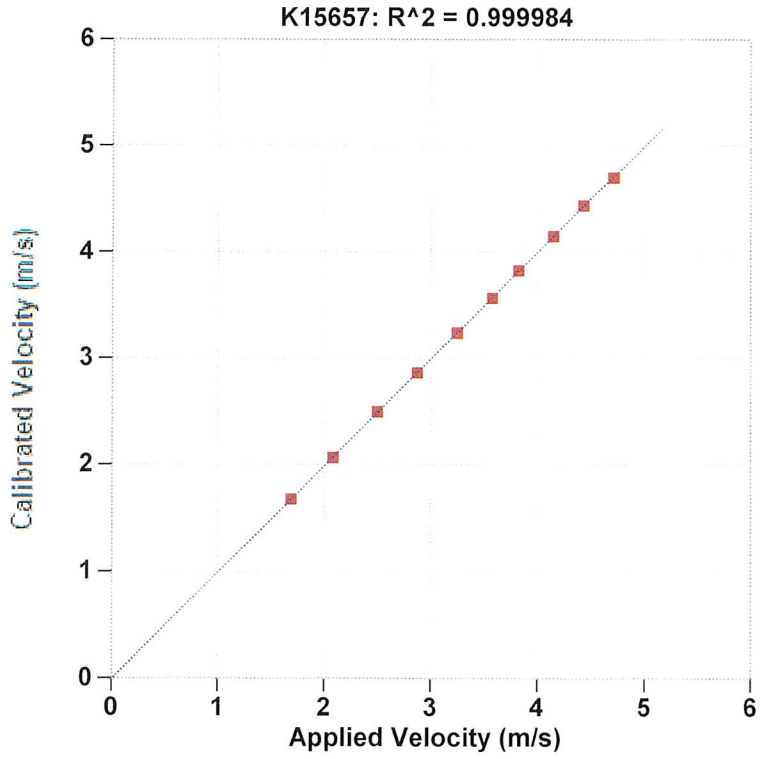

Reference Velocity	S/N K15657 Velocity
m/s	m/s
1.675	1.677
2.072	2.069
2.490	2.496
2.866	2.864
3.235	3.235
3.568	3.562
3.817	3.822
4.145	4.145
4.429	4.433
4.701	4.697

Maximum Acceleration: 1060 g's