

Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K2082 Temperature: 23.5 °C
Model: KICHER PR Humidity: 30%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

326.9 mv/5000g
(65.4 μ v/g)
R²: 0.999992 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 09Oct2026

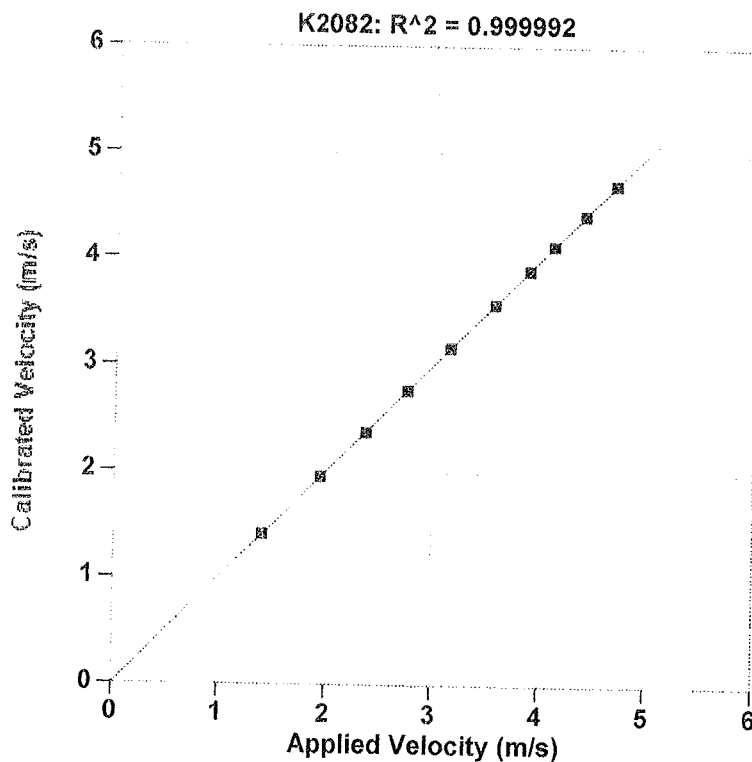

Reference Velocity	S/N K2082 Velocity
m/s	m/s
1.397	1.400
1.941	1.944
2.365	2.361
2.758	2.756
3.157	3.159
3.564	3.564
3.890	3.884
4.114	4.117
4.409	4.408
4.696	4.699
Maximum Acceleration: 1014 g's	