

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K2096 Temperature: 23.1 °C
Model: KICHER PR Humidity: 38%
Calibrated on: Channel 4 on 8G 5161 LE


PDA CALIBRATION FACTOR

318.0 mv/5000g
(63.6 μv/g)
R^2: 0.999977 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 15Oct2026

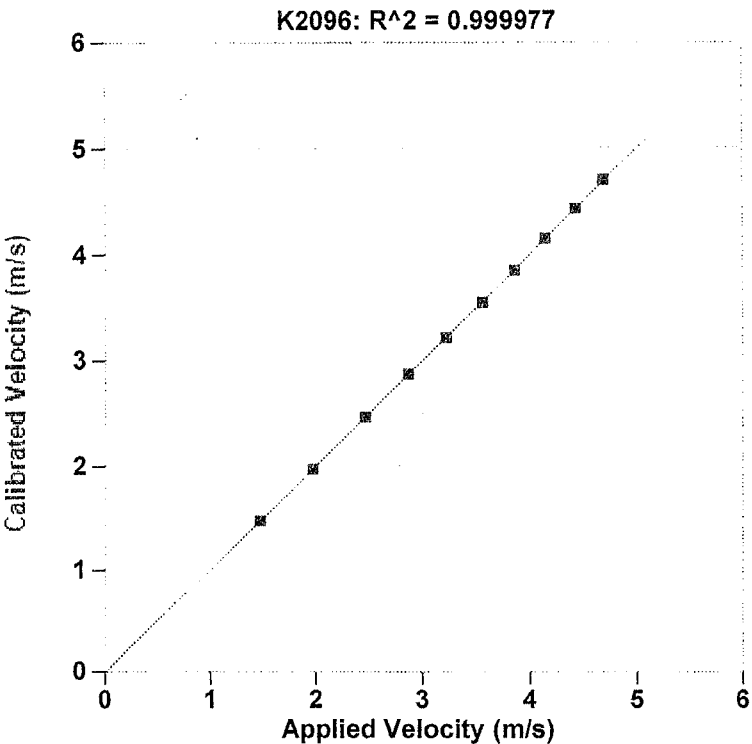

Reference Velocity	S/N K2096 Velocity
m/s	m/s
1.472	1.476
1.970	1.969
2.461	2.460
2.868	2.867
3.217	3.215
3.555	3.548
3.850	3.848
4.148	4.147
4.430	4.427
4.689	4.701
Maximum Acceleration: 1043 g's	