


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

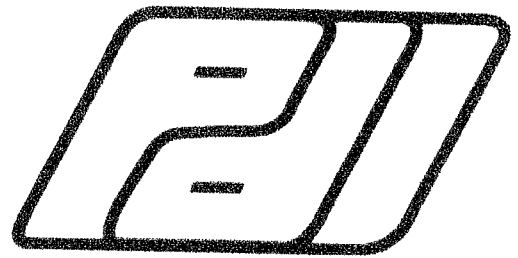

Serial No: K2263 Temperature: 23.5 °C

Model: KICHER PR Humidity: 29%

Calibrated on: Channel 4 on 8G 5161 LE

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).


PDA CALIBRATION FACTOR

341.5 mv/5000g

(68.3 μ v/g)


R²: 0.999990 [Chip programmed]

Operator: William Johnson

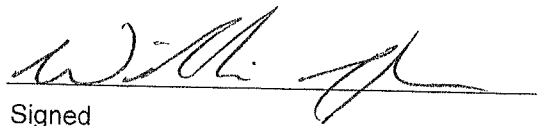
Signed

Calibration valid 2 years

From: 09Oct2026

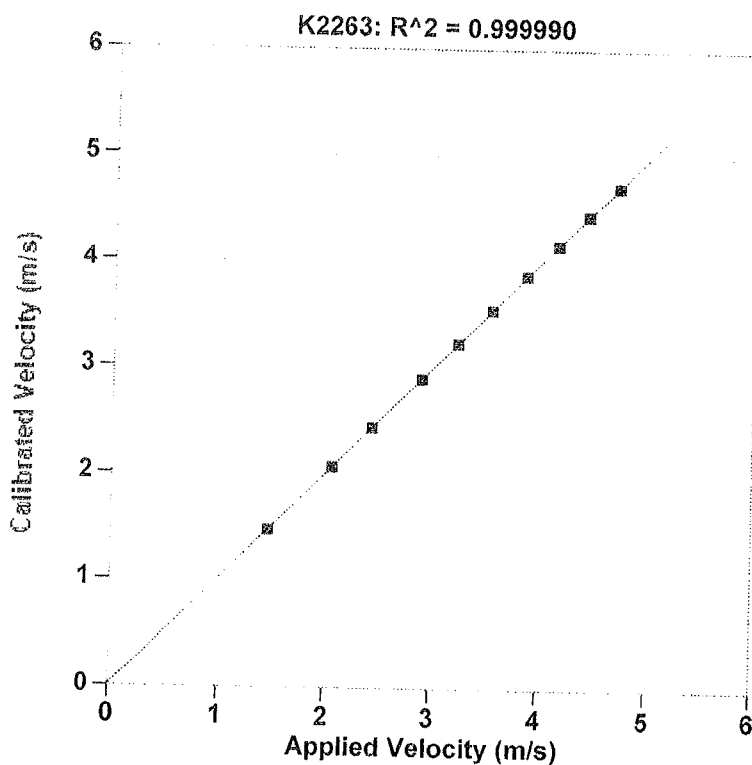

Reference Velocity	S/N K2263 Velocity
m/s	m/s
1.467	1.460
2.060	2.059
2.432	2.428
2.893	2.890
3.227	3.227
3.541	3.541
3.866	3.868
4.156	4.157
4.436	4.438
4.706	4.709

Maximum Acceleration: 1021 g's