

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.




Serial No: K3480 Temperature: 23.5 °C
Model: KICHER PR Humidity: 29%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

333.4 mv/5000g
(66.7 µv/g)
R^2: 0.999944 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 09Oct2026

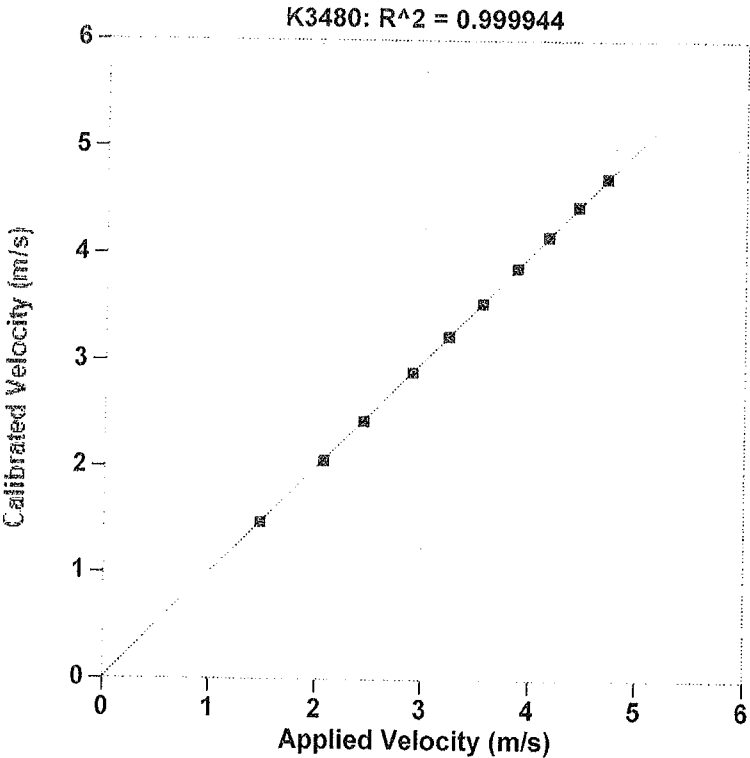

Reference Velocity	S/N K3480 Velocity
m/s	m/s
1.467	1.463
2.060	2.050
2.432	2.422
2.893	2.883
3.227	3.226
3.541	3.535
3.866	3.866
4.156	4.163
4.436	4.445
4.706	4.714
Maximum Acceleration: 1021 g's	