


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

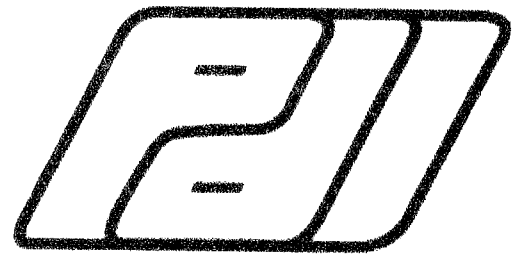


Serial No: K490 Temperature: 23.3 °C
Model: KICHER PR Humidity: 38%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

295.1 mv/5000g
(59.0 μ v/g)
R²: 0.999993 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 15Oct2026

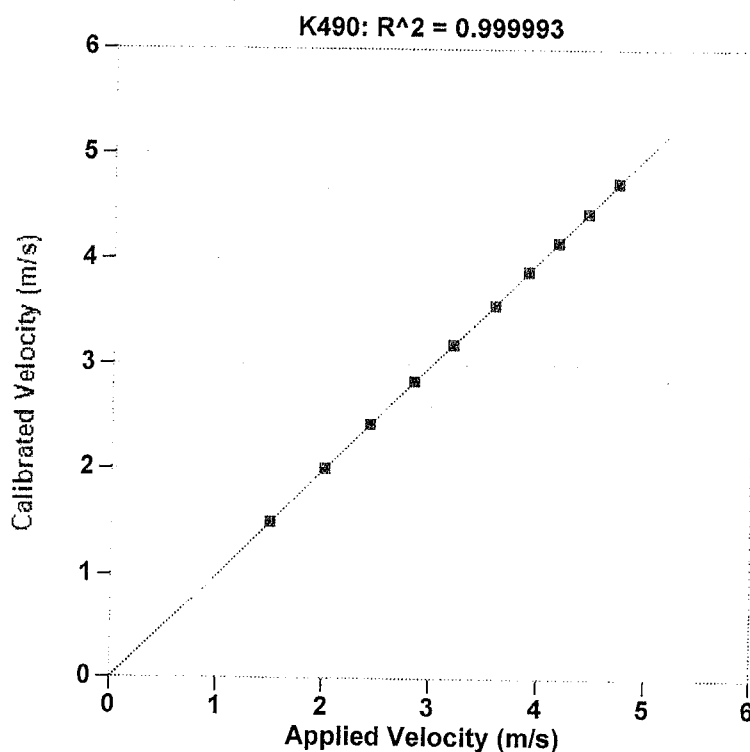

Reference Velocity	S/N K490 Velocity
m/s	m/s
1.496	1.499
2.008	2.008
2.429	2.429
2.838	2.840
3.198	3.197
3.579	3.572
3.891	3.892
4.169	4.167
4.445	4.449
4.733	4.734
Maximum Acceleration: 1057 g's	