


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

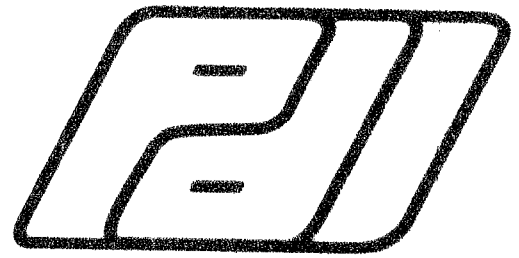

Serial No: K5131 Temperature: 21.8 °C

Model: KICHER PR Humidity: 41%

Calibrated on: Channel 3 on 8G 5161 LE

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

340.7 mv/5000g

(68.1 μ v/g)


R²: 0.999982 [Chip programmed]

Operator: William Johnson

William Johnson
Signed

Calibration valid 2 years

From: 26Sep2026

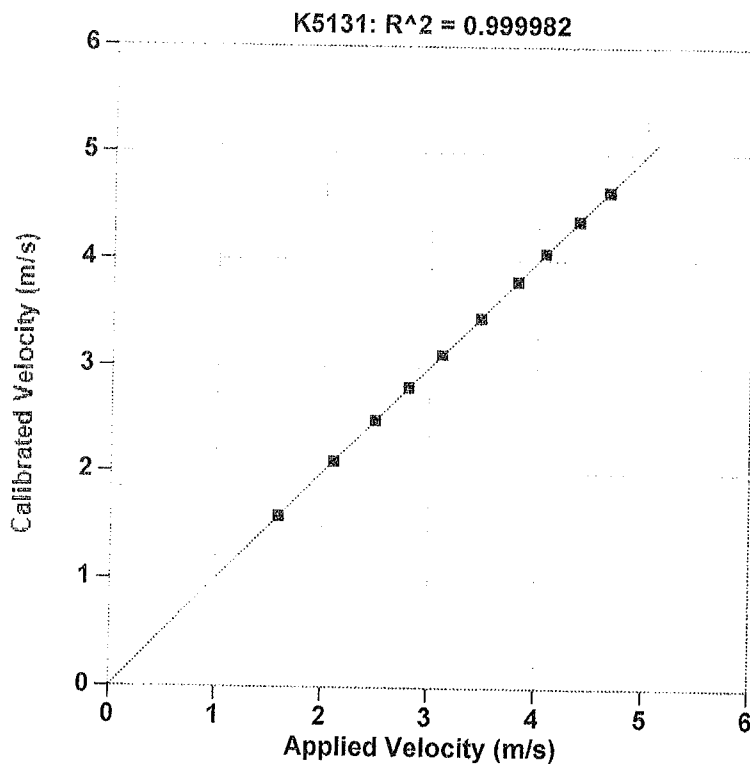

Reference Velocity	S/N K5131 Velocity
m/s	m/s
1.580	1.583
2.106	2.100
2.491	2.495
2.805	2.809
3.112	3.119
3.470	3.468
3.812	3.810
4.073	4.074
4.381	4.382
4.664	4.659
Maximum Acceleration: 1014 g's	