


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

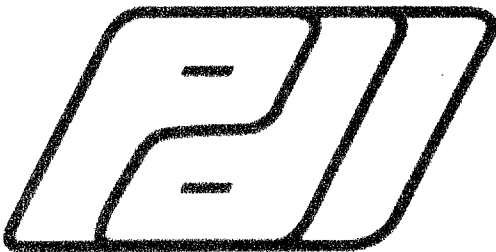

Serial No: K6189 Temperature: 23.1 °C
Model: KICHER PR Humidity: 39%
Calibrated on: Channel 3 on 8G 5161 LE


PDA CALIBRATION FACTOR

378.0 mv/5000g
(75.6 μv/g)
R^2: 0.999983 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Operator: William Johnson


Signed

Calibration valid 2 years

From: 15Oct2026

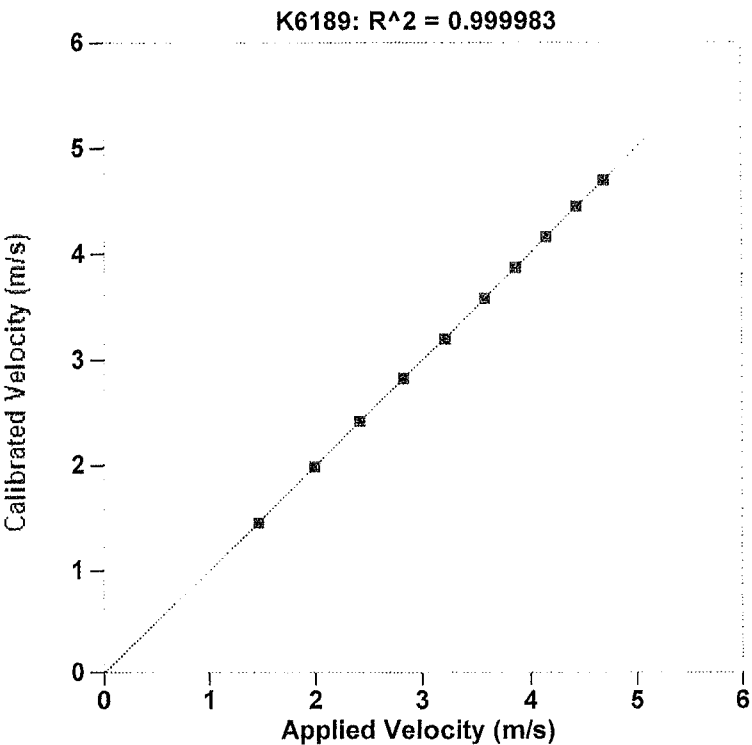

Reference Velocity	S/N K6189 Velocity
m/s	m/s
1.461	1.456
1.993	1.986
2.418	2.417
2.829	2.825
3.205	3.200
3.578	3.578
3.863	3.864
4.152	4.152
4.438	4.443
4.687	4.693
Maximum Acceleration: 1043 g's	