
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: W346
PDI Gage Factor: 93.1
Mean Linear Correlation Coefficient: 0.999935

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2027.6	-6.298	433.1	1.358
-1614.2	-5.059	807.1	2.494
-1168.0	-3.701	1161.4	3.603
-675.9	-2.172	1528.9	4.697
-288.7	-0.936	1863.5	5.734
65.6	0.198	2003.5	6.129

Calibration Curve

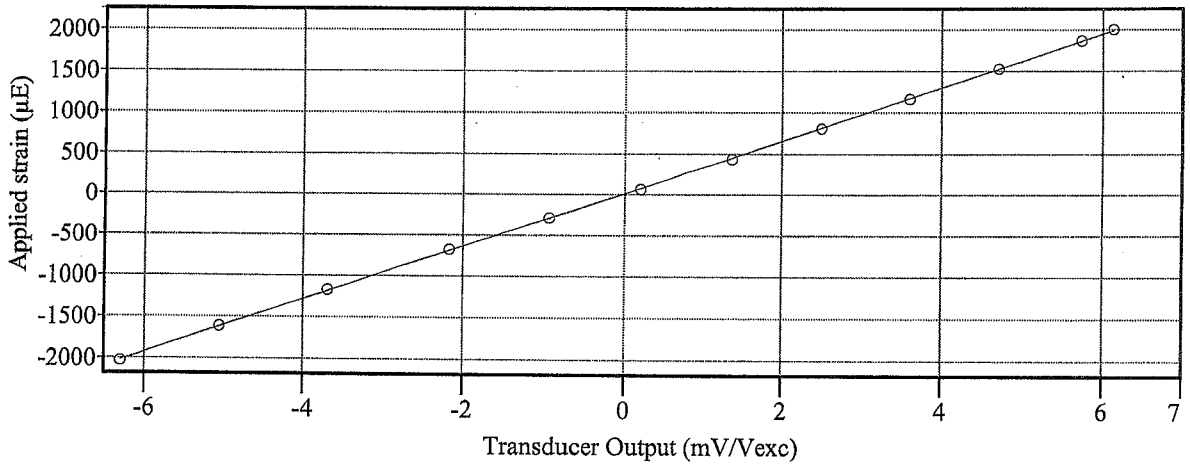

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: W346
Calibration Date: 10/1/2026 1:05:47 PM
Calibration valid 2 years

Pile Dynamics, Inc.