
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: X785
PDI Gage Factor: 92.4
Mean Linear Correlation Coefficient: 0.999968

Table 1: Representative Calibration Data

Applied strain (µE)	Gage Output (mV/Vexc)	Applied strain (µE)	Gage Output (mV/Vexc)
-1909.4	-5.892	393.7	1.331
-1528.9	-4.692	767.7	2.495
-1126.4	-3.468	1135.2	3.647
-682.4	-2.103	1496.1	4.752
-321.5	-0.935	1843.8	5.825
32.8	0.188	1981.6	6.233

Calibration Curve

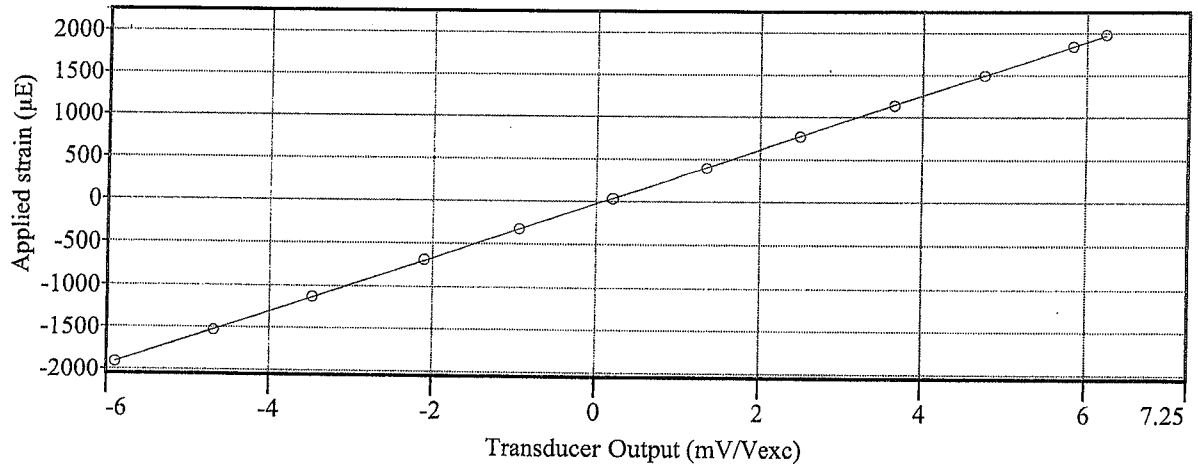

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: X785

Calibration Date: 10/13/2026 9:36:37 AM

Calibration valid 2 years

Pile Dynamics, Inc.