
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 050D
PDI Gage Factor: 138.5
Mean Linear Correlation Coefficient: 0.999985

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2001.3	-4.195	452.8	0.941
-1509.2	-3.158	813.6	1.699
-1063.0	-2.202	1128.6	2.361
-741.5	-1.546	1456.7	3.045
-367.5	-0.768	1791.3	3.719
45.9	0.103	1988.2	4.138

Calibration Curve

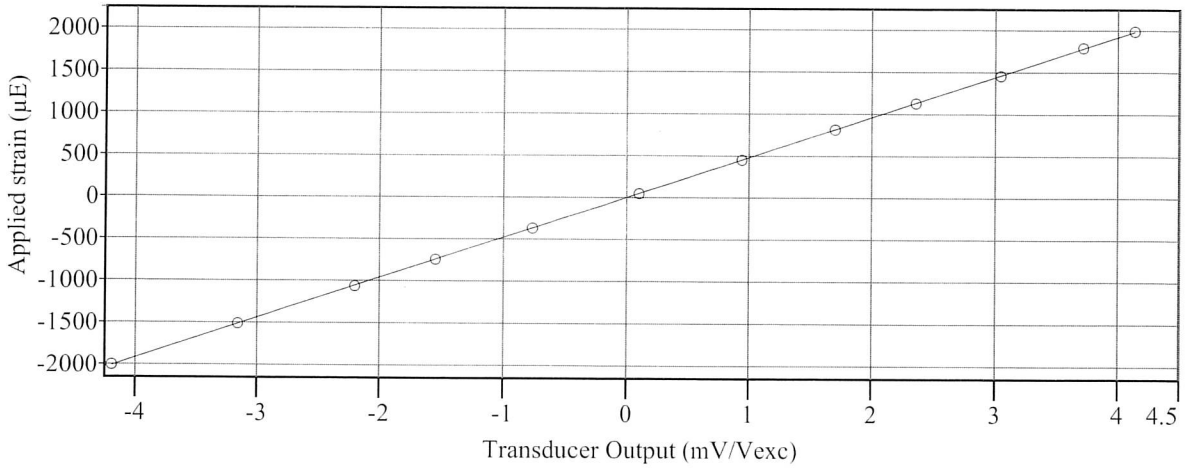

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: Kelly Beal

PDI Gage: 050D

Calibration Date: NOV 0 6 2026

Calibration valid 2 years

Pile Dynamics, Inc.