Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 078C
PDI Gage Factor: 145.9
Mean Linear Correlation Coefficient: 0.999902

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2336.0	-4.721	511.8	0.994
-1771.7	-3.568	826.8	1.622
-1194.2	-2.406	1168.0	2.274
-769.9	-1.562	1509.2	2.927
-354.3	-0.726	1857.0	3.587
120.3	0.215	2007.9	3.897

Calibration Curve

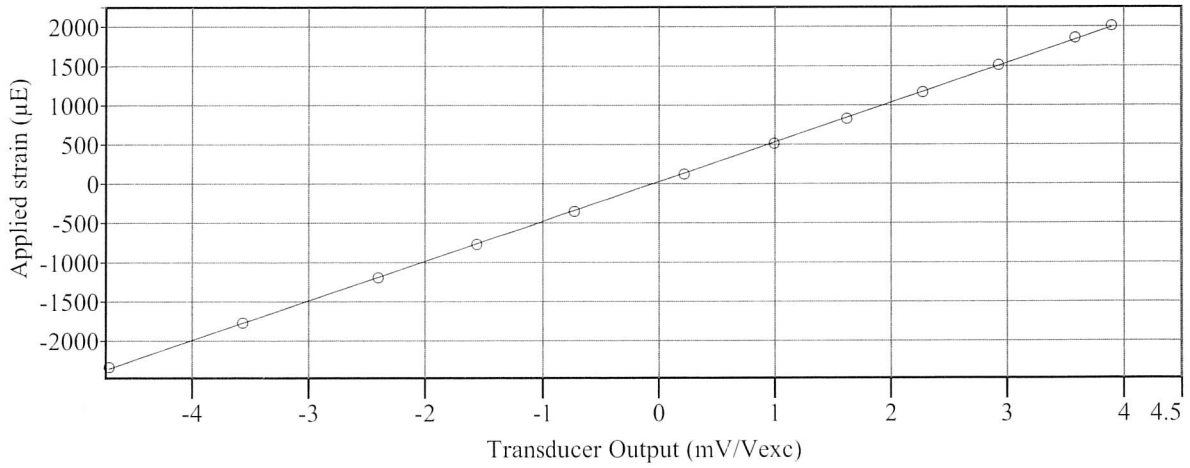

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 078C

Calibration Date: NOV 04 2026

Calibration valid 2 years

Pile Dynamics, Inc.