
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 226D
PDI Gage Factor: 93.8
Mean Linear Correlation Coefficient: 0.999981

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2021.0	-6.261	728.3	2.242
-1437.0	-4.467	1043.3	3.209
-859.6	-2.686	1378.0	4.218
-419.9	-1.304	1706.0	5.229
-32.8	-0.115	2007.9	6.126
400.3	1.221		

Calibration Curve

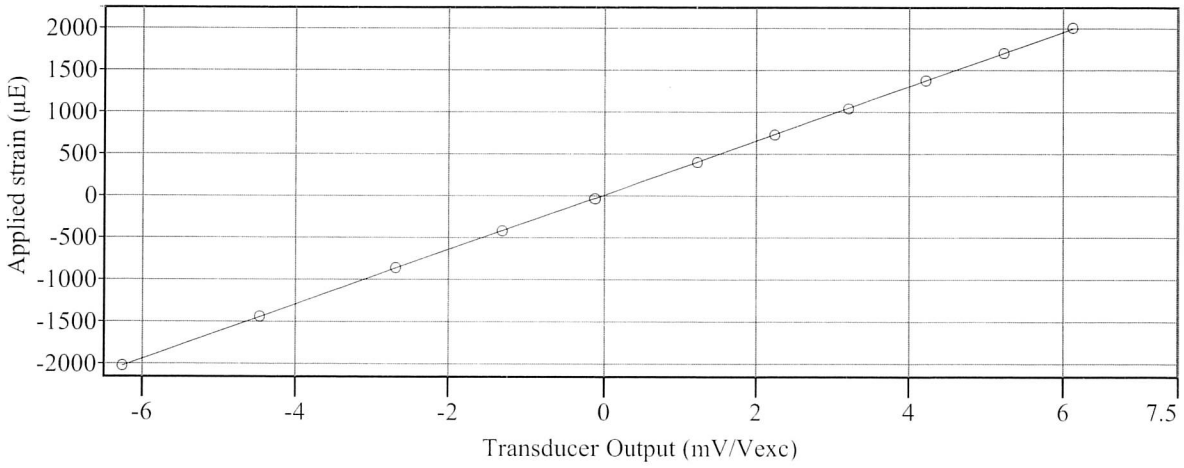

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 226D

Calibration Date: NOV 0 9 2026

Calibration valid 2 years

Pile Dynamics, Inc.