Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 232D
PDI Gage Factor: 95.1
Mean Linear Correlation Coefficient: 0.999969

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2007.9	-6.008	728.3	2.288
-1434.8	-4.296	1036.7	3.245
-859.6	-2.577	1371.4	4.238
-406.8	-1.183	1699.5	5.239
-39.4	-0.076	2012.2	6.144
393.7	1.256		

Calibration Curve

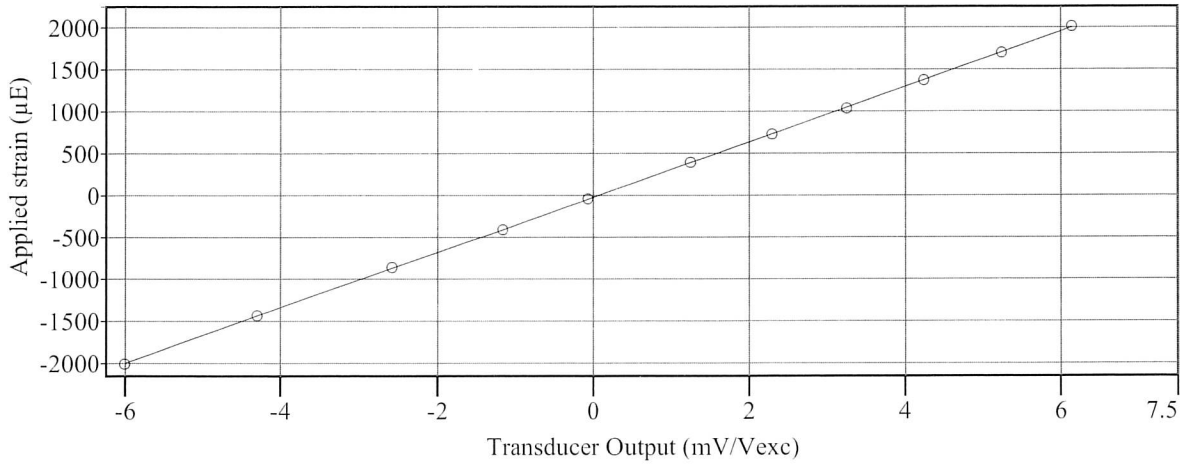

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 232D

Calibration Date: NOV 16 2026

Calibration valid 2 years

Pile Dynamics, Inc.