
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 244D
PDI Gage Factor: 94.2
Mean Linear Correlation Coefficient: 0.999965

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1587.9	-4.870	590.6	1.827
-1128.6	-3.477	857.4	2.656
-767.7	-2.354	1141.7	3.514
-472.4	-1.461	1419.5	4.361
-105.0	-0.318	1692.9	5.195
269.0	0.829	1992.6	6.057

Calibration Curve

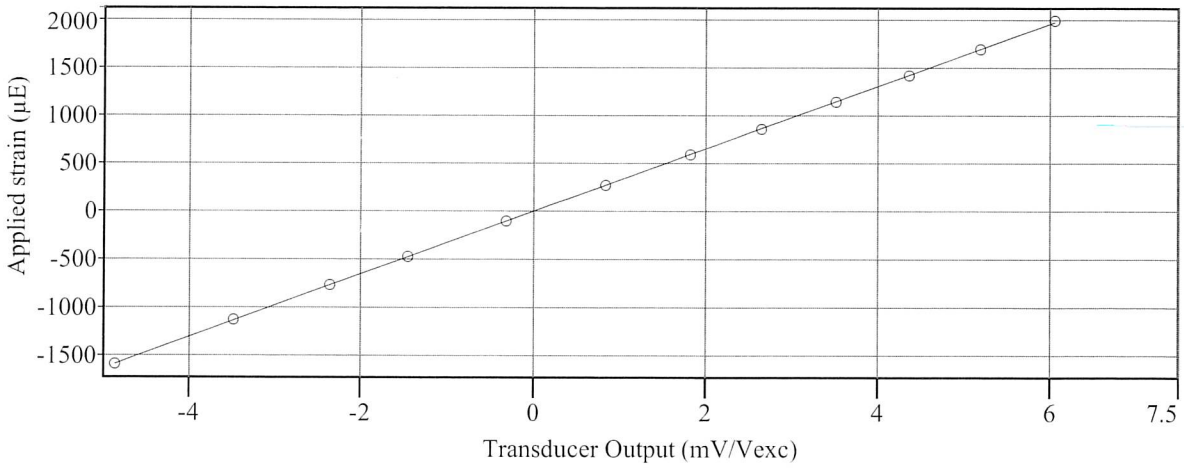

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 244D

Calibration Date: NOV 05 2026

Calibration valid 2 years

Pile Dynamics, Inc.