
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 245D
PDI Gage Factor: 94.7
Mean Linear Correlation Coefficient: 0.999884

Table 1: Representative Calibration Data

Applied strain (µE)	Gage Output (mV/Vexc)	Applied strain (µE)	Gage Output (mV/Vexc)
-2329.4	-7.000	505.2	1.603
-1778.2	-5.408	837.7	2.639
-1194.2	-3.678	1187.7	3.711
-780.8	-2.392	1542.0	4.776
-367.5	-1.107	1909.4	5.827
118.1	0.381	2016.6	6.129

Calibration Curve

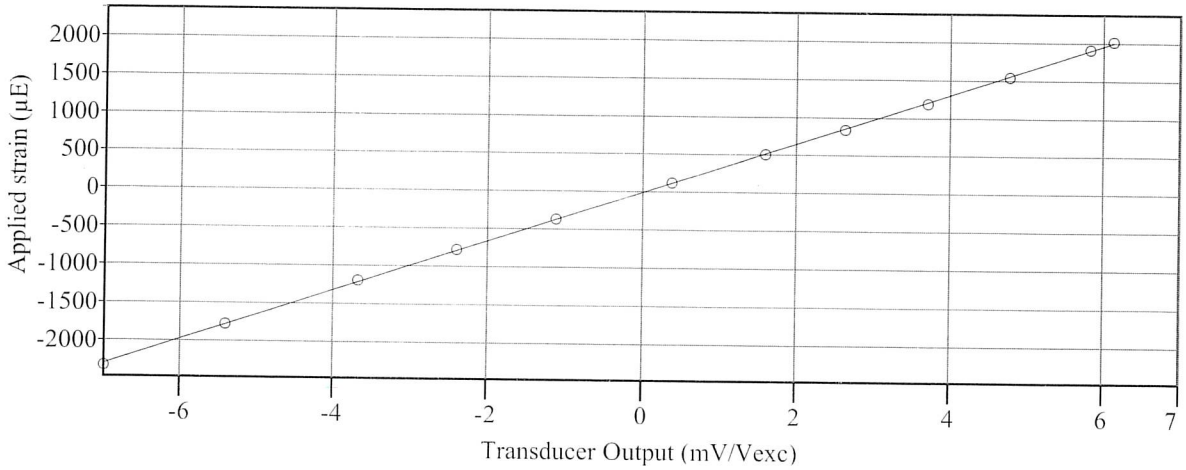

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: Kelly Beal

PDI Gage: 245D

Calibration Date: NOV 06 2026

Calibration valid 2 years

Pile Dynamics, Inc.