
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 282D
PDI Gage Factor: 93.1
Mean Linear Correlation Coefficient: 0.999990

Table 1: Representative Calibration Data

Applied strain (µE)	Gage Output (mV/Vexc)	Applied strain (µE)	Gage Output (mV/Vexc)
-1883.2	-5.828	439.6	1.386
-1417.3	-4.382	761.2	2.390
-958.0	-2.963	1049.9	3.281
-656.2	-2.026	1345.1	4.210
-321.5	-0.992	1644.8	5.129
59.1	0.211	2007.9	6.224

Calibration Curve

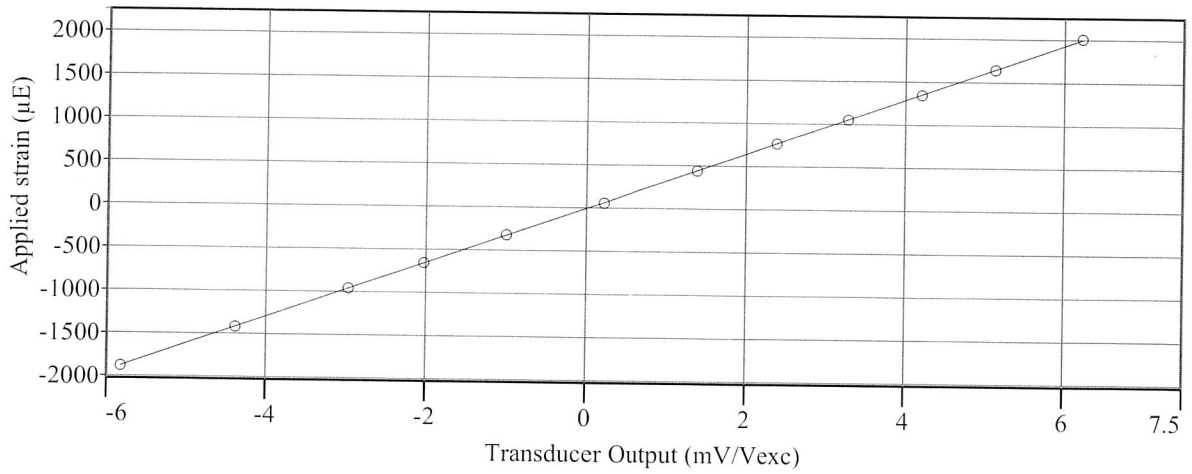

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: Kelly Beal

PDI Gage: 282D

Calibration Date: NOV 16 2026

Calibration valid 2 years

Pile Dynamics, Inc.