Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 298D
PDI Gage Factor: 93.2
Mean Linear Correlation Coefficient: 0.999975

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1863.5	-5.808	721.8	2.227
-1395.5	-4.354	997.4	3.101
-958.0	-3.002	1292.7	4.009
-669.3	-2.107	1587.9	4.906
-334.6	-1.043	1876.6	5.774
56.9	0.152	1988.2	6.106
419.9	1.302		

Calibration Curve

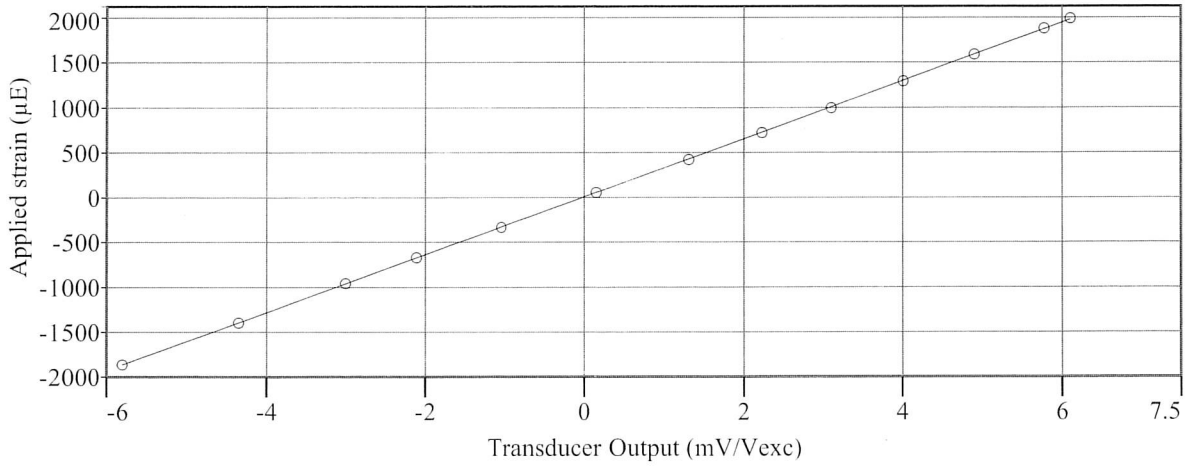

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 298D

Calibration Date: NOV 17 2026

Calibration valid 2 years

Pile Dynamics, Inc.