Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	50824	**Temperature:**	23.1 °C
Model:	PE	**Humidity:**	30%
Calibrated on:	Channel 3 on 8G 5161 LE		

PDA CALIBRATION FACTOR

995.7 g's/volt

R^2: 0.999966 [Chip programmed]

Operator: William Johnson


Signed

Calibration valid 2 years

From: 22Oct2026

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

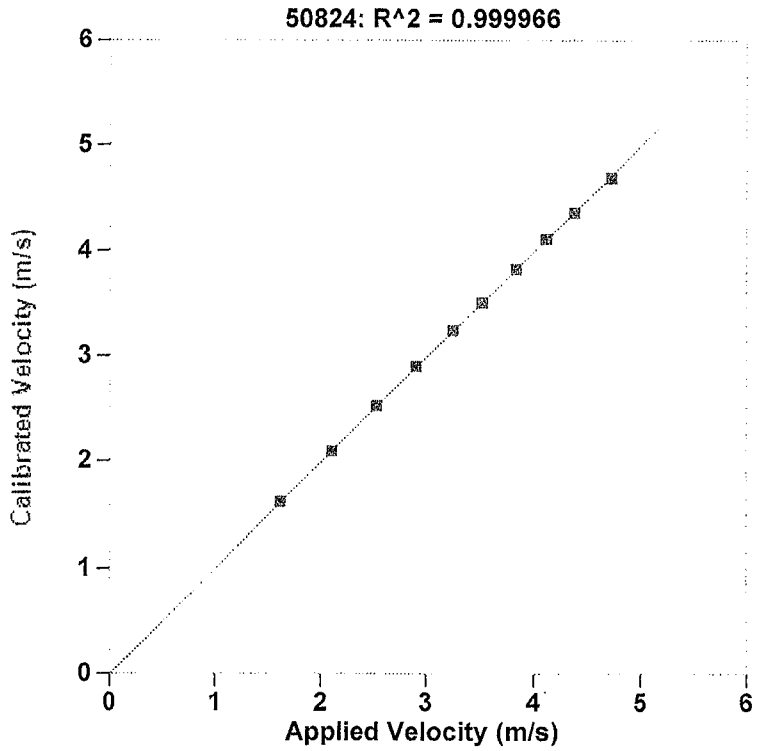

Reference Velocity	S/N 50824 Velocity
m/s	m/s
1.614	1.618
2.100	2.097
2.524	2.530
2.901	2.908
3.244	3.250
3.512	3.514
3.830	3.830
4.113	4.115
4.372	4.369
4.710	4.697

Maximum Acceleration: 1063 g's