
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 982C
PDI Gage Factor: 142.4
Mean Linear Correlation Coefficient: 0.999969

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1994.8	-4.060	371.8	0.759
-1496.1	-3.054	636.5	1.298
-1010.5	-2.065	896.8	1.832
-590.6	-1.197	1174.5	2.380
-343.4	-0.688	1452.3	2.937
19.7	0.042	2001.3	4.028

Calibration Curve

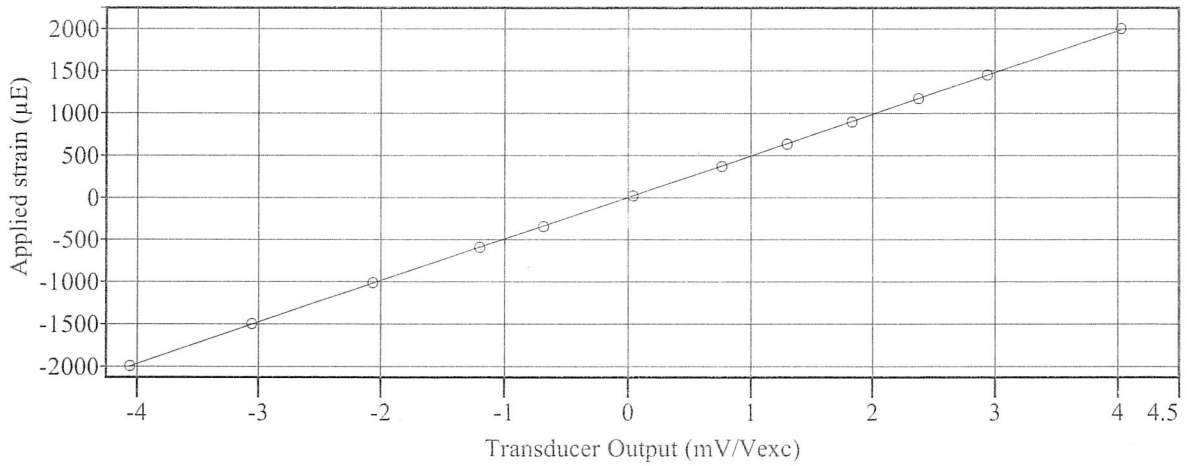

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 982C

Calibration Date: NOV 0 6 2026

Calibration valid 2 years

Pile Dynamics, Inc.