Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K10723	**Temperature:**	22.6 °C
Model:	KICHER PR	**Humidity:**	34%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

399.3 mv/5000g
(79.9 µv/g)
R^2: 0.999948 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: 29Oct2026

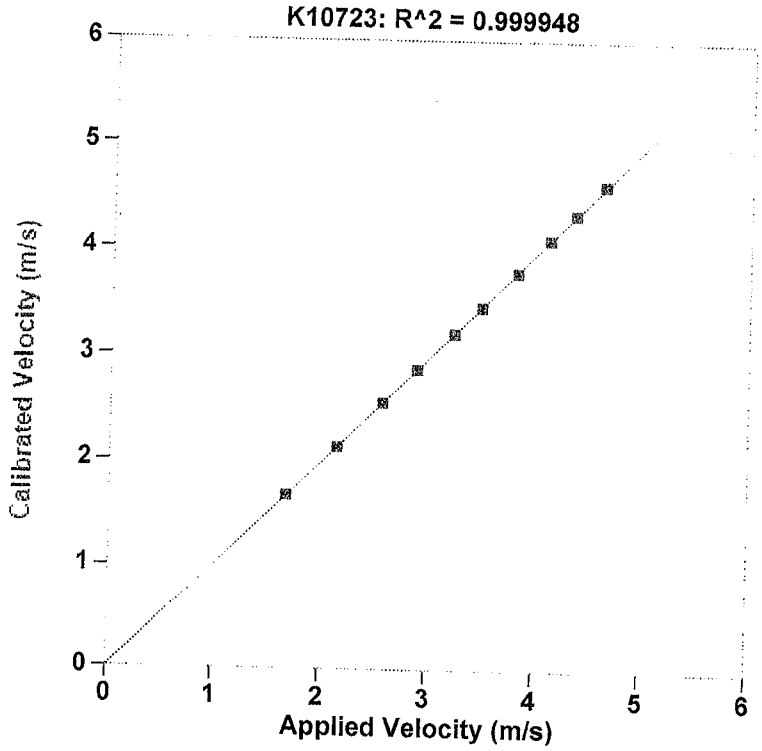

Reference Velocity	S/N K10723 Velocity
m/s	m/s
1.673	1.677
2.139	2.140
2.561	2.560
2.880	2.878
3.223	3.221
3.475	3.470
3.813	3.801
4.111	4.109
4.353	4.355
4.623	4.638

Maximum Acceleration: 1046 g's