Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15556	**Temperature:**	21.0 °C
Model:	KICHER PR	**Humidity:**	56%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

386.0 mv/5000g
(77.2 µv/g)
R^2: 0.999983 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 17 2026

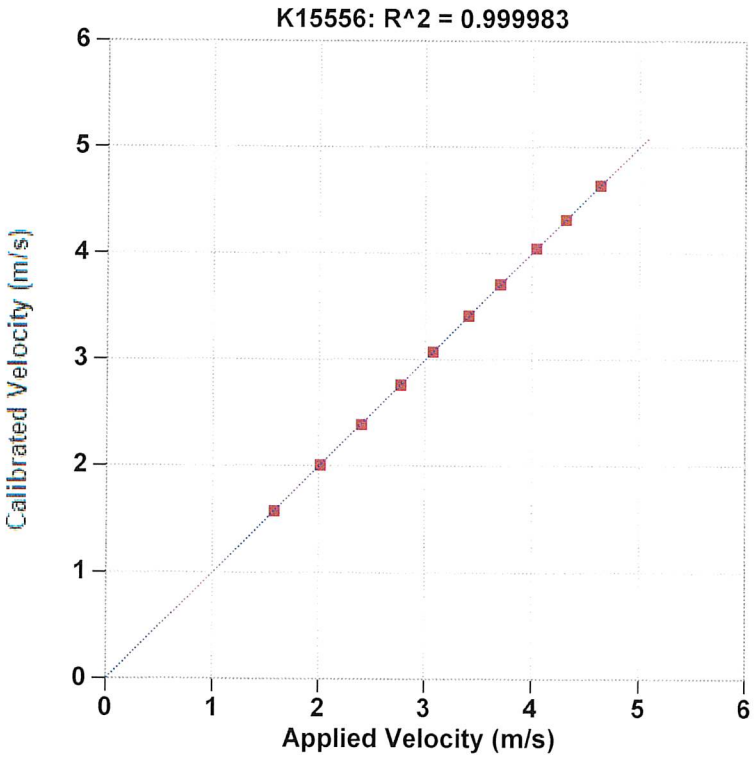

Reference Velocity	S/N K15556 Velocity
m/s	m/s
1.581	1.578
2.015	2.009
2.398	2.390
2.766	2.762
3.073	3.075
3.410	3.412
3.709	3.709
4.040	4.043
4.312	4.314
4.637	4.640

Maximum Acceleration: 988 g's