Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15560	**Temperature:**	21.0 °C
Model:	KICHER PR	**Humidity:**	56%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


404.3 mv/5000g
(80.9 µv/g)
R^2: 0.999962 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 19 2026

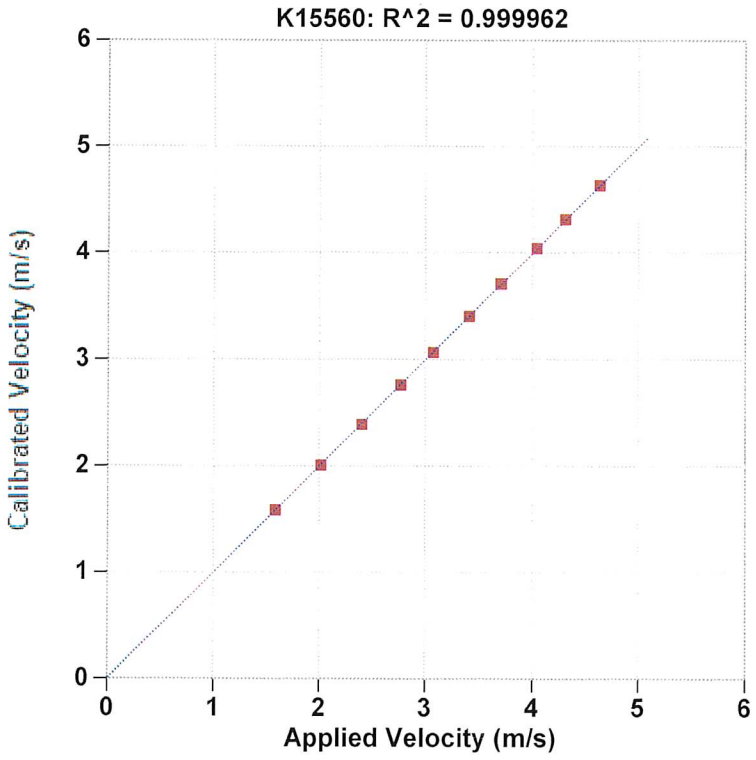

Reference Velocity	S/N K15560 Velocity
m/s	m/s
1.581	1.581
2.015	2.004
2.398	2.390
2.766	2.762
3.073	3.067
3.410	3.407
3.709	3.714
4.040	4.046
4.312	4.318
4.637	4.639

Maximum Acceleration: 988 g's