Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15565	**Temperature:**	23.5 °C
Model:	KICHER PR	**Humidity:**	37%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


385.5 mv/5000g
(77.1 µv/g)
R^2: 0.999990 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 2 2026

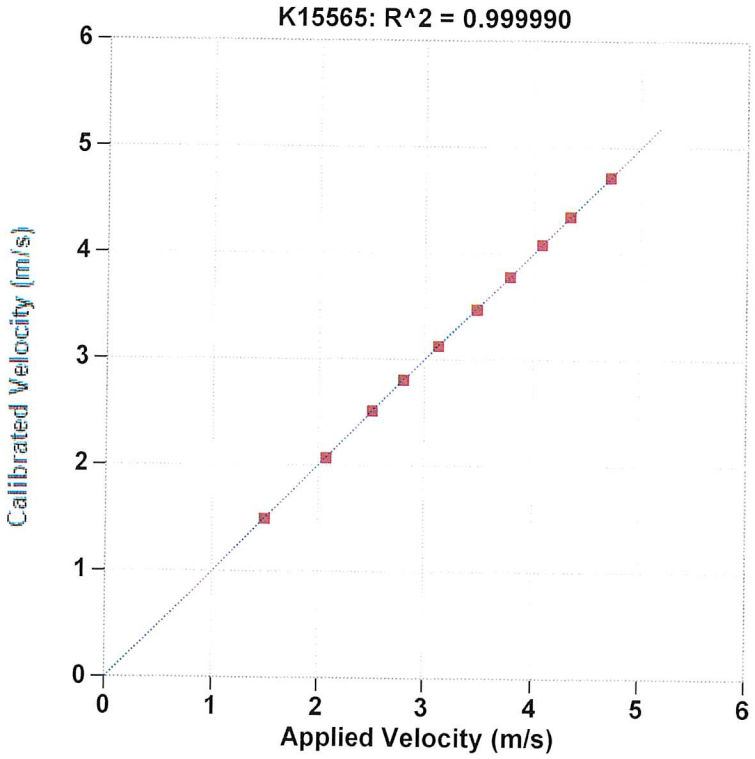

Reference Velocity	S/N K15565 Velocity
m/s	m/s
1.496	1.491
2.069	2.066
2.509	2.512
2.803	2.802
3.123	3.124
3.475	3.470
3.778	3.778
4.079	4.083
4.343	4.347
4.717	4.716

Maximum Acceleration: 1018 g's