Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15596	**Temperature:**	23.5 °C
Model:	KICHER PR	**Humidity:**	42%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

414.0 mv/5000g
(82.8 µv/g)
R^2: 0.999963 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 04 2026

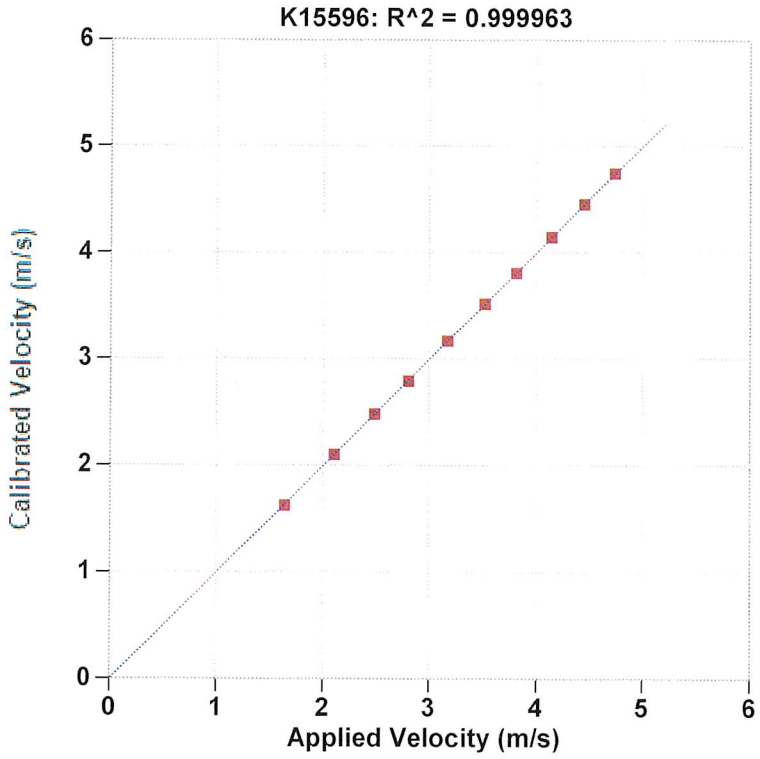

Reference Velocity	S/N K15596 Velocity
m/s	m/s
1.634	1.625
2.103	2.099
2.482	2.480
2.802	2.790
3.170	3.170
3.512	3.514
3.809	3.806
4.138	4.146
4.451	4.454
4.741	4.745

Maximum Acceleration: 1026 g's